

Certificate of Calibration

Pile Dynamics, Inc.



Calibrated by Pile Dynamics, Inc.

Serial No: 84836 Temperature: 23.3 °C
 Model: PE Humidity: 36%
 Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR
907.3 g's/volt
 R²: 0.999954 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
 958 g's/volt
 Ref Acc 2: 85363! Cal on: 14Nov2025
 1000 g's/volt


Operator: William Johnson

Signed

Calibration valid 2 years

From: MAR 05 2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

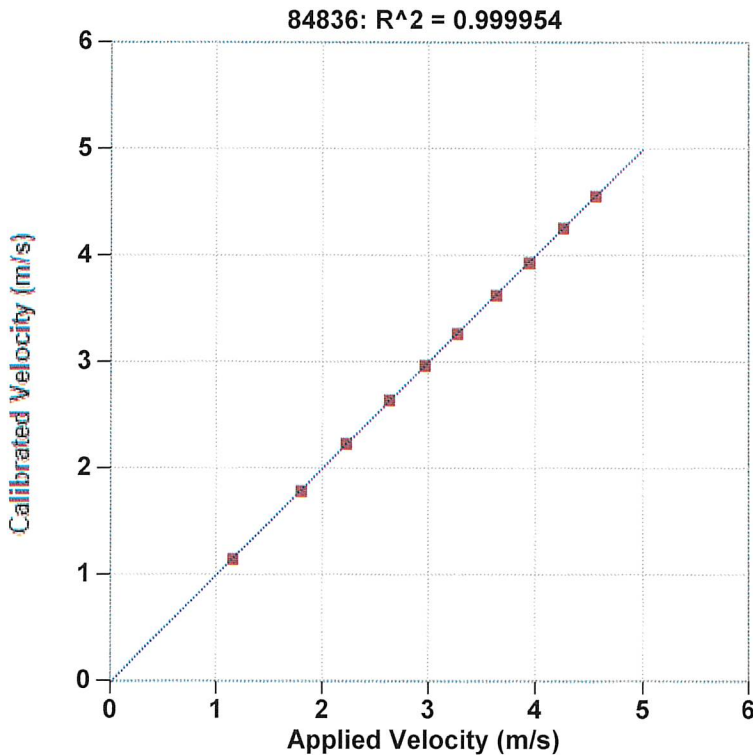

| Reference Velocity | S/N 84836 Velocity |
|--------------------|--------------------|
| m/s | m/s |
| 1.156 | 1.151 |
| 1.796 | 1.792 |
| 2.226 | 2.238 |
| 2.630 | 2.644 |
| 2.965 | 2.968 |
| 3.273 | 3.271 |
| 3.638 | 3.630 |
| 3.945 | 3.937 |
| 4.263 | 4.264 |
| 4.564 | 4.565 |

Maximum Acceleration: 984 g's