


# Pile Dynamics, Inc.

## Transducer G497

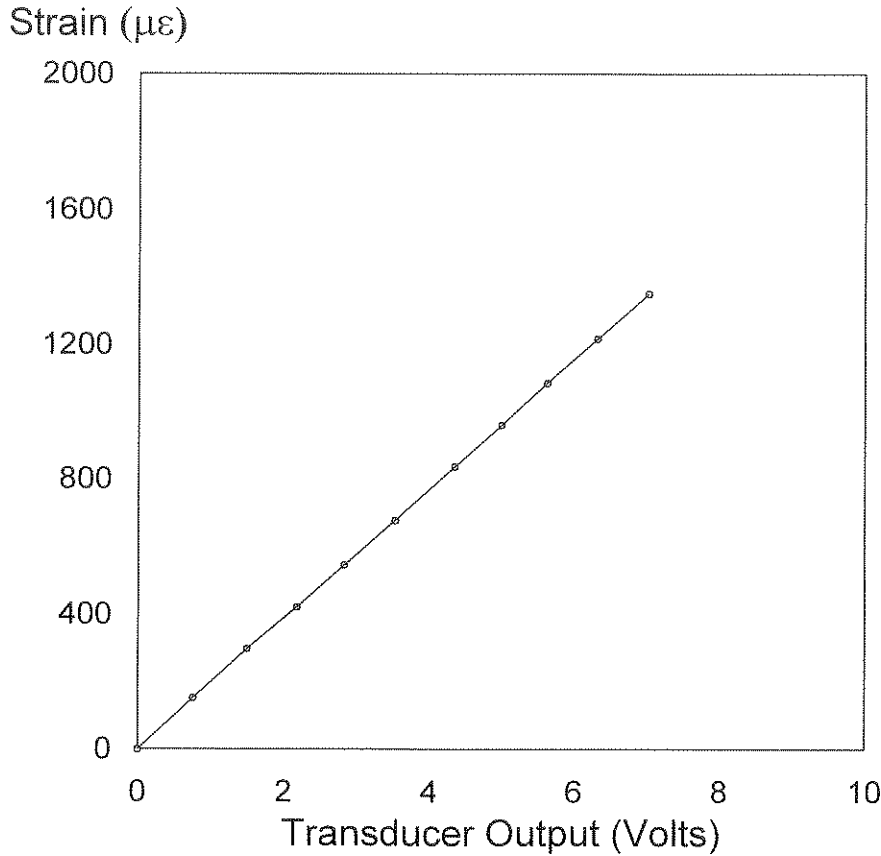

PDA Cal Factor (5.0 V) 95.9 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
153	0.75
297	1.49
421	2.17
544	2.82
676	3.52
836	4.34
960	4.99
1086	5.62
1218	6.31
1351	7.02

Shunt (60.4 K $\Omega$ ) 2.5 V  
 General Factor 332.9 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by: *Rob B. Smith*  
 Calibrated on: 05-May-2011

Smart Sensor?  Yes  No Smart Chip Programmed by: VT on: 5-10-11 CRC value 92 D8