




Pile Dynamics, Inc.

Transducer G500

Strain ($\mu\epsilon$)

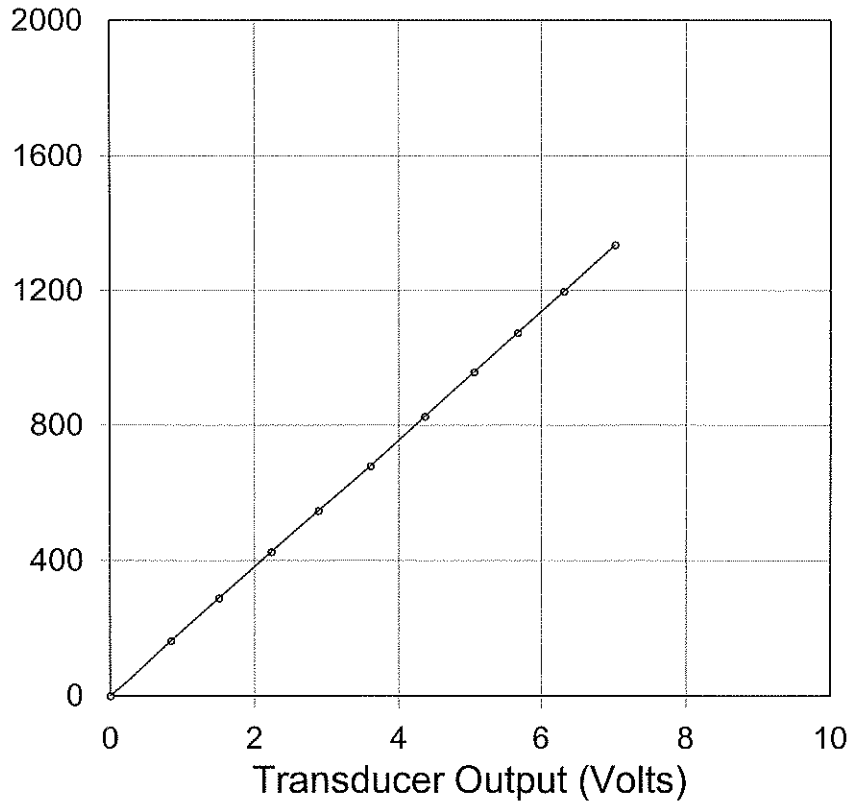

PDA Cal Factor (5.0 V)

94.7 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
164	0.83
290	1.50
426	2.23
547	2.89
679	3.60
825	4.36
958	5.05
1074	5.66
1197	6.31
1336	7.02


Shunt (60.4 K Ω)
General Factor

2.5 V
328.8 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by:
Calibrated on:


20-Apr-2011