




Pile Dynamics, Inc.

Transducer G505

Strain ($\mu\epsilon$)

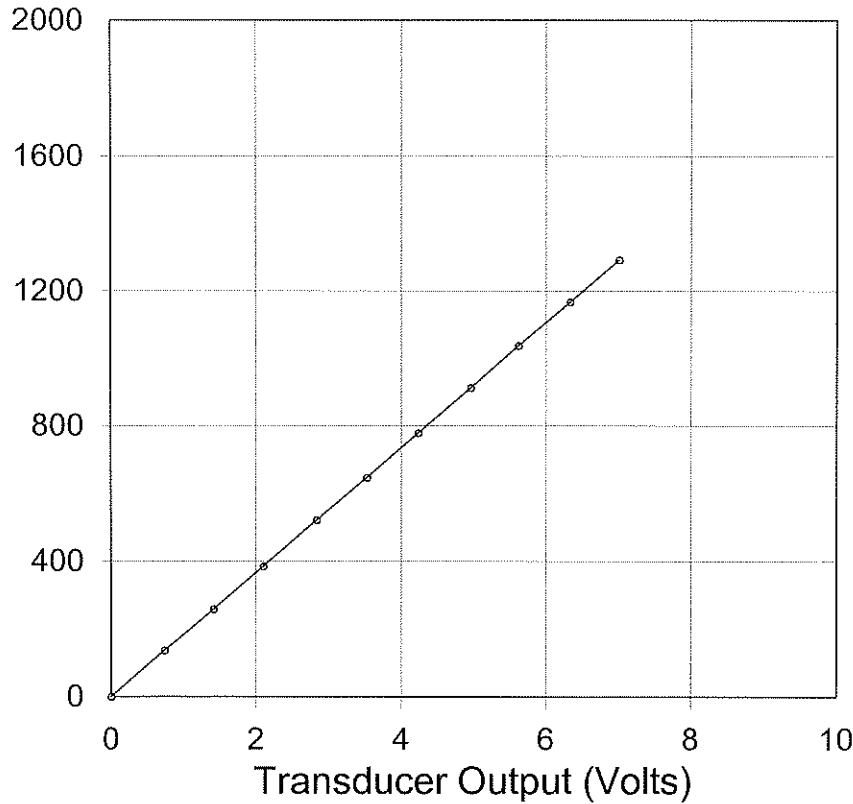

PDA Cal Factor (5.0 V)

92.2 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
137	0.74
258	1.41
385	2.10
520	2.83
645	3.52
777	4.23
912	4.96
1037	5.62
1167	6.33
1293	7.01

Shunt (60.4 K Ω)

2.5 V

General Factor

320.1 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

14-Apr-2011