




Pile Dynamics, Inc.

Transducer G506

Strain ($\mu\epsilon$)

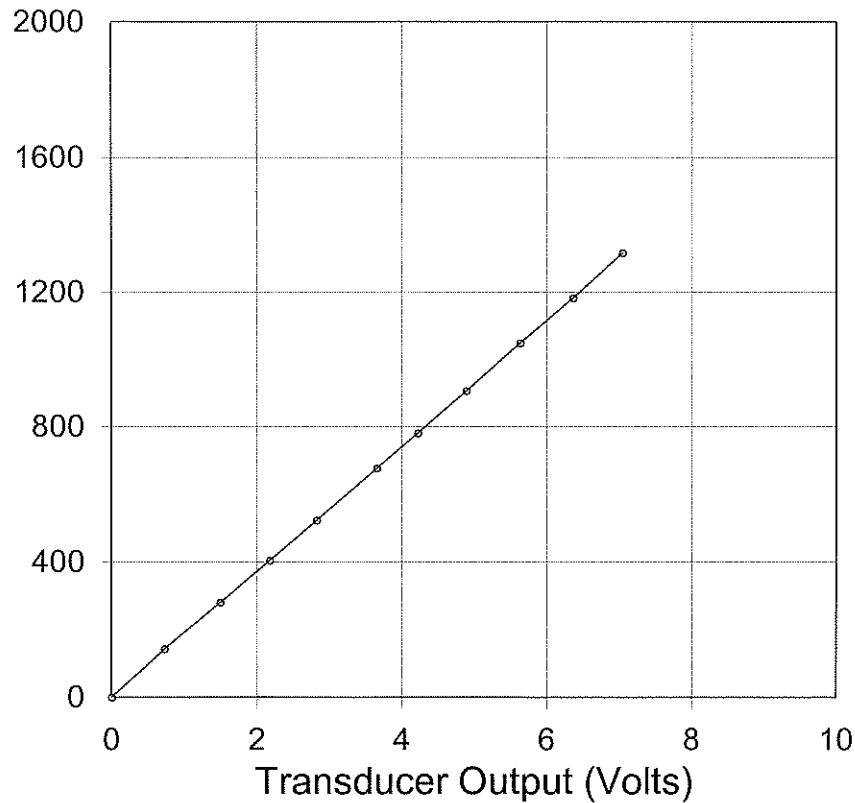

PDA Cal Factor (5.0 V)

93.0 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
144	0.72
280	1.49
404	2.17
522	2.82
677	3.65
780	4.22
905	4.89
1049	5.63
1183	6.36
1318	7.04

Shunt (60.4 K Ω)

2.5 V

General Factor

322.8 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

20-Apr-2011