


Pile Dynamics, Inc.

Transducer G507

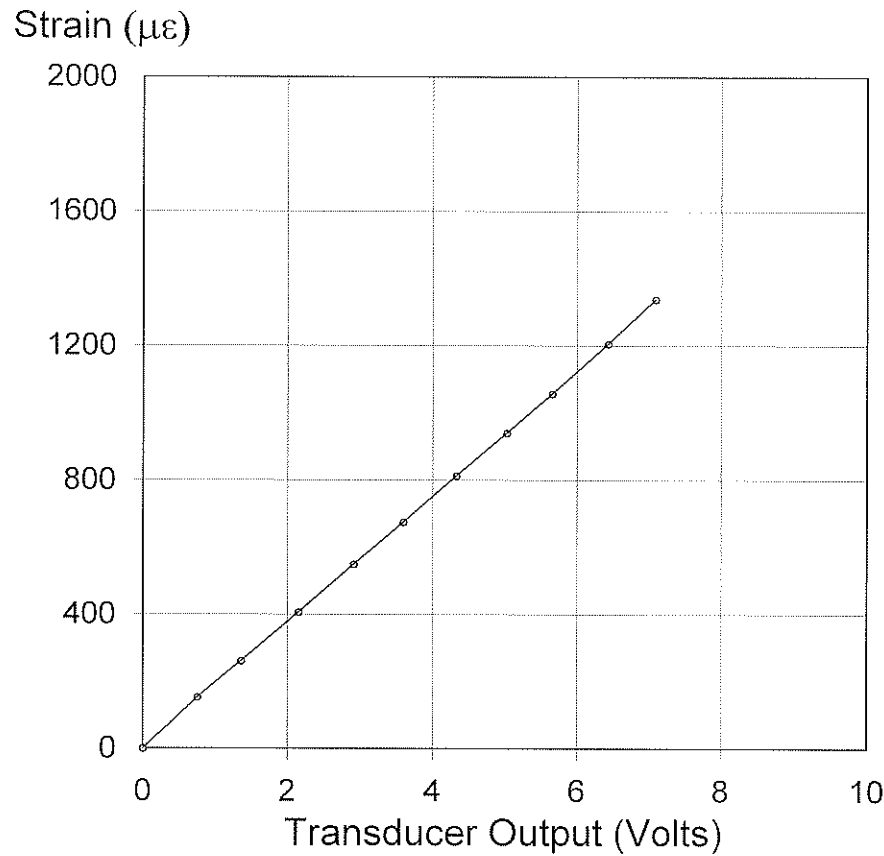


PDA Cal Factor (5.0 V) 93.6 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
152	0.75
262	1.36
406	2.15
549	2.91
675	3.60
813	4.32
941	5.02
1058	5.65
1207	6.43
1338	7.09

Shunt (60.4 K Ω) 2.5 V
 General Factor 324.9 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by: 
 Calibrated on: 10-Aug-2011