


Pile Dynamics, Inc.

Transducer G508

Strain ($\mu\epsilon$)

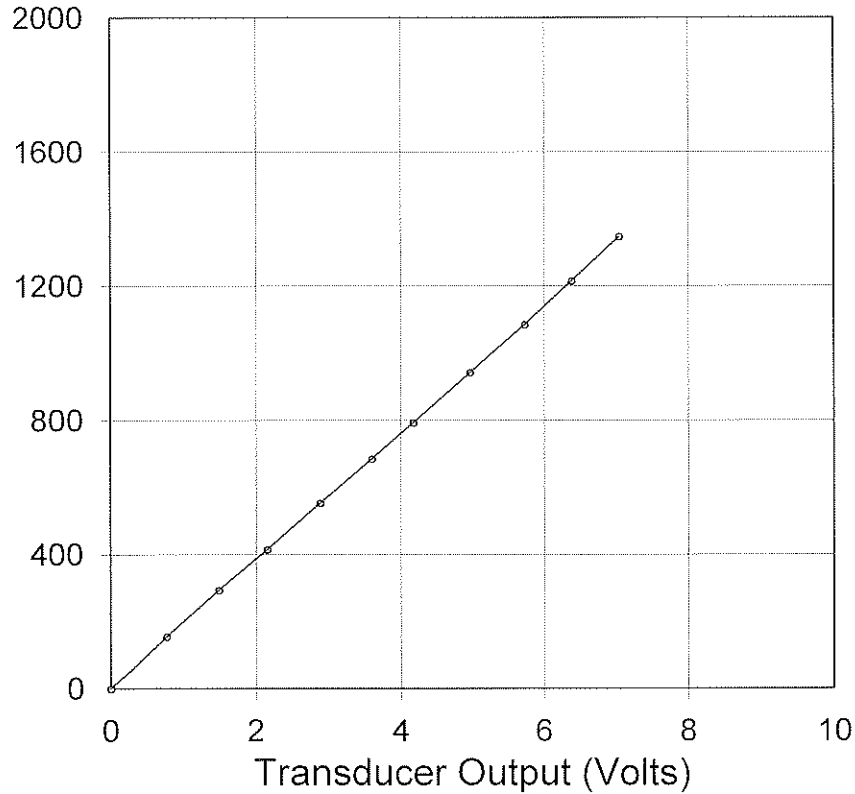

PDA Cal Factor (5.0 V)

94.6 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
155	0.76
293	1.48
415	2.15
554	2.89
685	3.59
793	4.17
943	4.96
1086	5.72
1215	6.39
1346	7.04

Shunt (60.4 K Ω)

2.5 V


General Factor

328.6 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:


13-Sep-2011