




Pile Dynamics, Inc.

Transducer G509

Strain ($\mu\epsilon$)

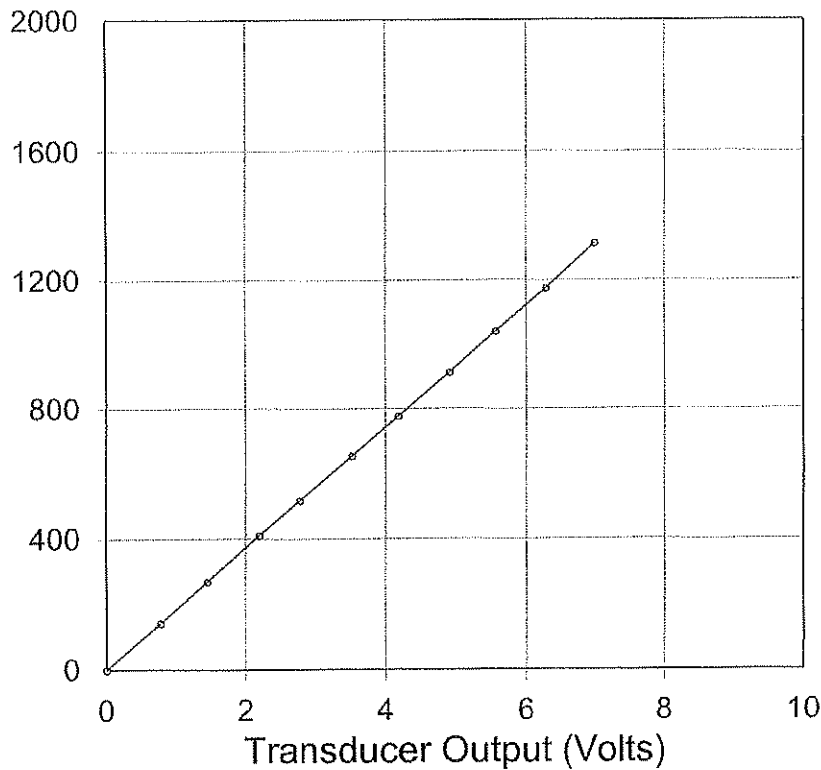

PDA Cal Factor (5.0 V)

93.6 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
144	0.76
269	1.44
410	2.19
515	2.78
652	3.52
775	4.18
912	4.90
1040	5.56
1174	6.28
1315	6.99

Shunt (60.4 K Ω)

2.5 V

General Factor

325.0 $\mu\epsilon$ /mV/V

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by:

Calibrated on:

13-Apr-2011