




Pile Dynamics, Inc.

Transducer G510

Strain ($\mu\epsilon$)

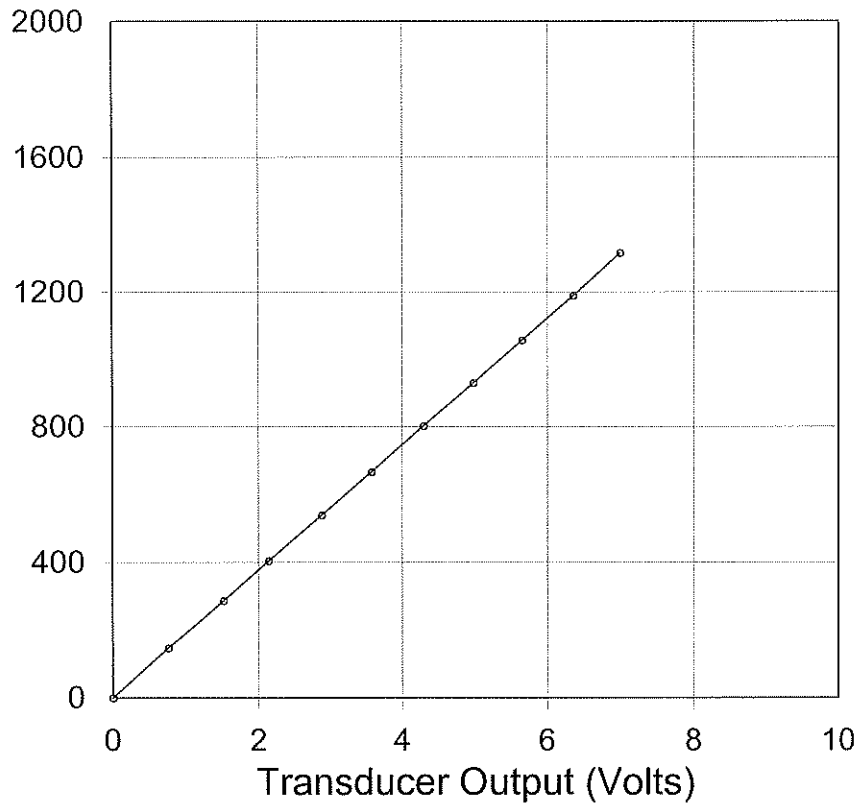

PDA Cal Factor (5.0 V)

93.5 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
148	0.75
287	1.51
403	2.14
538	2.88
666	3.57
802	4.29
930	4.98
1058	5.65
1190	6.35
1318	7.00

Shunt (60.4 K Ω)

2.5 V

General Factor

324.7 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

15-Apr-2011