




Pile Dynamics, Inc.

Transducer G511

Strain ($\mu\epsilon$)

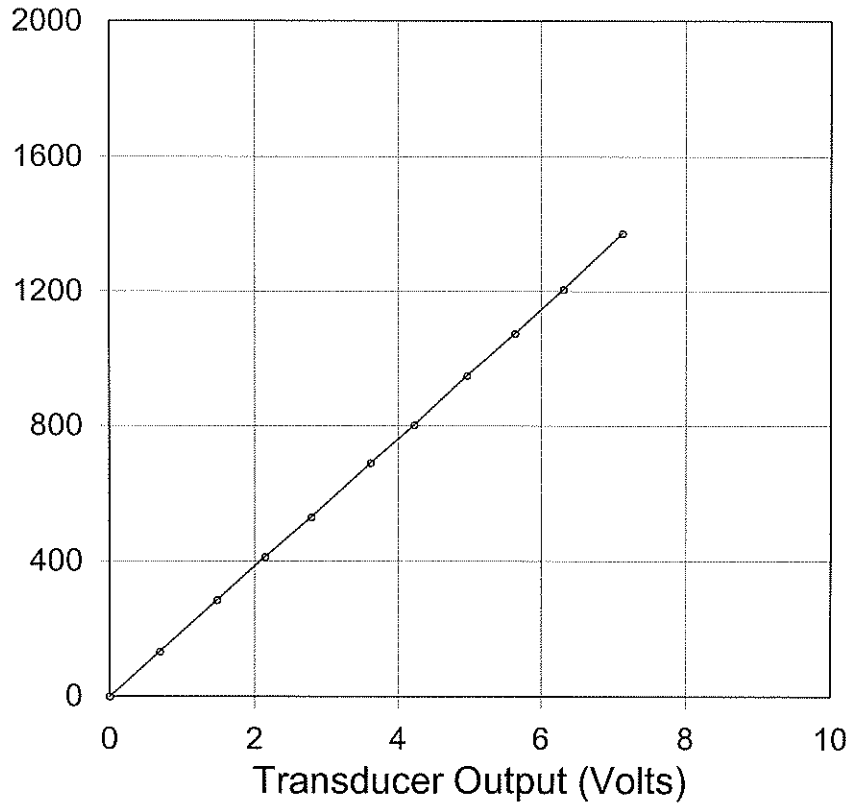

PDA Cal Factor (5.0 V)

95.7 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
132	0.68
285	1.47
413	2.14
529	2.77
689	3.62
803	4.22
949	4.96
1074	5.63
1206	6.30
1373	7.13

Shunt (60.4 K Ω)

2.5 V

General Factor

332.4 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

20-Apr-2011