




Pile Dynamics, Inc.

Transducer G514

Strain ($\mu\epsilon$)

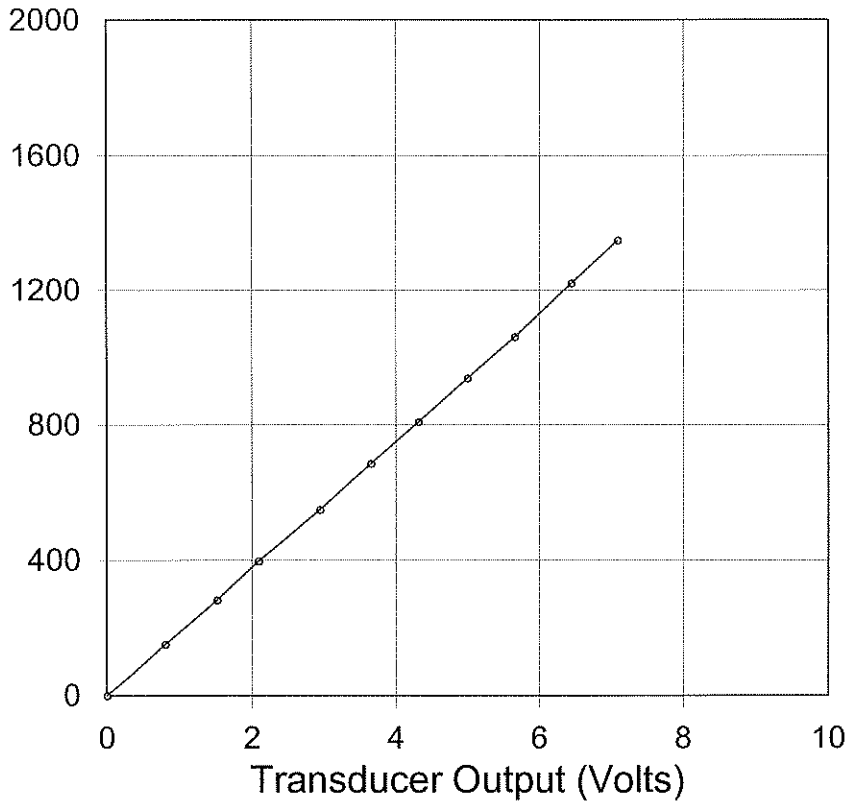

PDA Cal Factor (5.0 V)

94.7 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
153	0.80
283	1.51
397	2.09
549	2.94
684	3.65
809	4.31
939	4.99
1063	5.65
1222	6.44
1350	7.09

Shunt (60.4 K Ω)

2.5 V

General Factor

329.0 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by:

Calibrated on:

20-Apr-2011