




Pile Dynamics, Inc.

Transducer G515

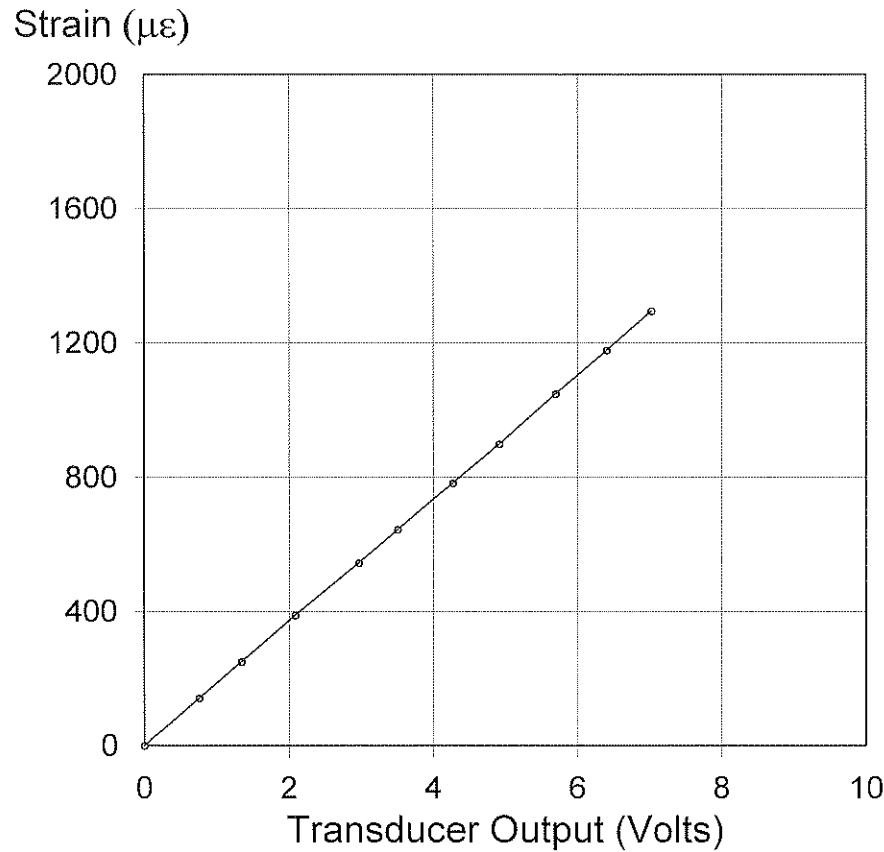

PDA Cal Factor (5.0 V) 91.9 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
143	0.75
250	1.34
388	2.08
545	2.96
644	3.50
782	4.26
899	4.91
1048	5.70
1179	6.40
1296	7.02

Shunt (60.4 K Ω) 2.5 V
 General Factor 319.0 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by: *Uttrak*
 Calibrated on: 18-Oct-2011