




Pile Dynamics, Inc.

Transducer G517

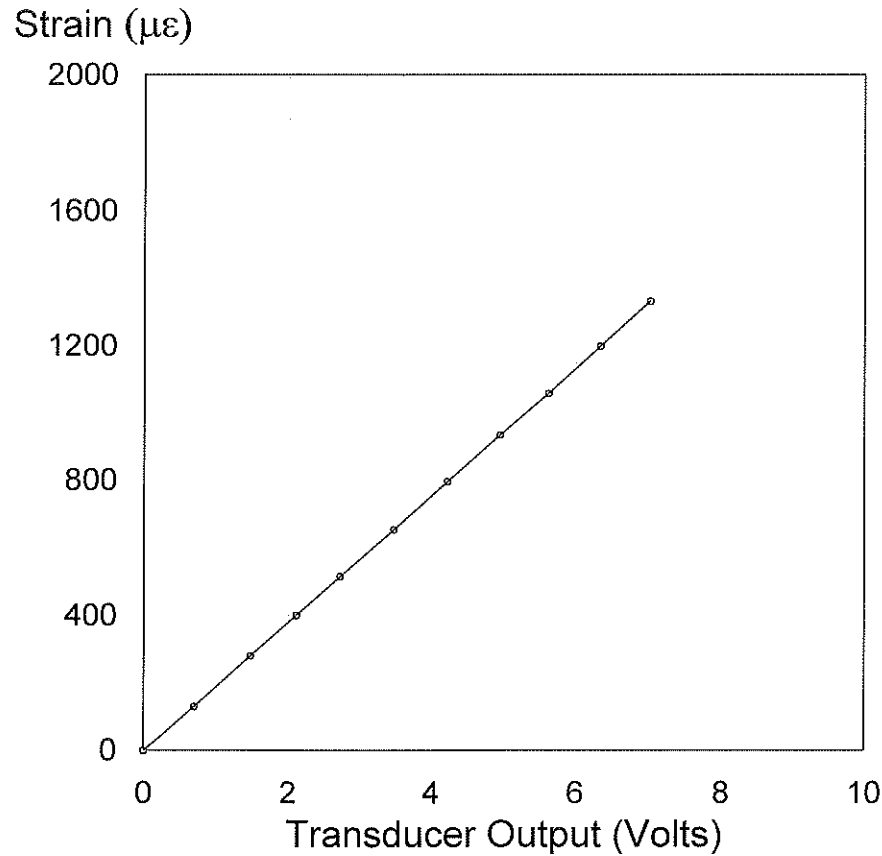

PDA Cal Factor (5.0 V) 94.6 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
130	0.69
281	1.47
399	2.11
513	2.72
652	3.47
796	4.22
933	4.95
1058	5.62
1198	6.33
1332	7.02

Shunt (60.4 K Ω) 2.5 V
 General Factor 328.3 $\mu\epsilon/mVV$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by: 
 Calibrated on: 18-May-2011