




# Pile Dynamics, Inc.

## Transducer G542

Strain ( $\mu\epsilon$ )

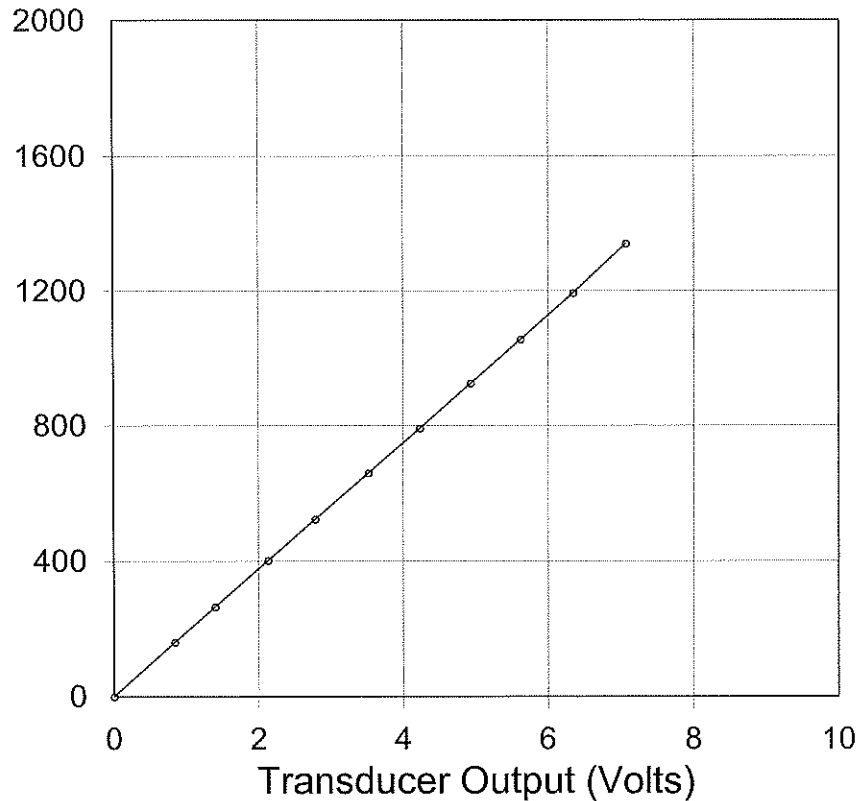

PDA Cal Factor (5.0 V)

94.2 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
162	0.83
264	1.39
401	2.13
522	2.78
659	3.52
791	4.23
926	4.93
1056	5.62
1195	6.34
1341	7.07

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

327.1 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

18-Apr-2011