




Pile Dynamics, Inc.

Pile Dynamics, Inc.

Transducer

G544

Strain ($\mu\epsilon$)

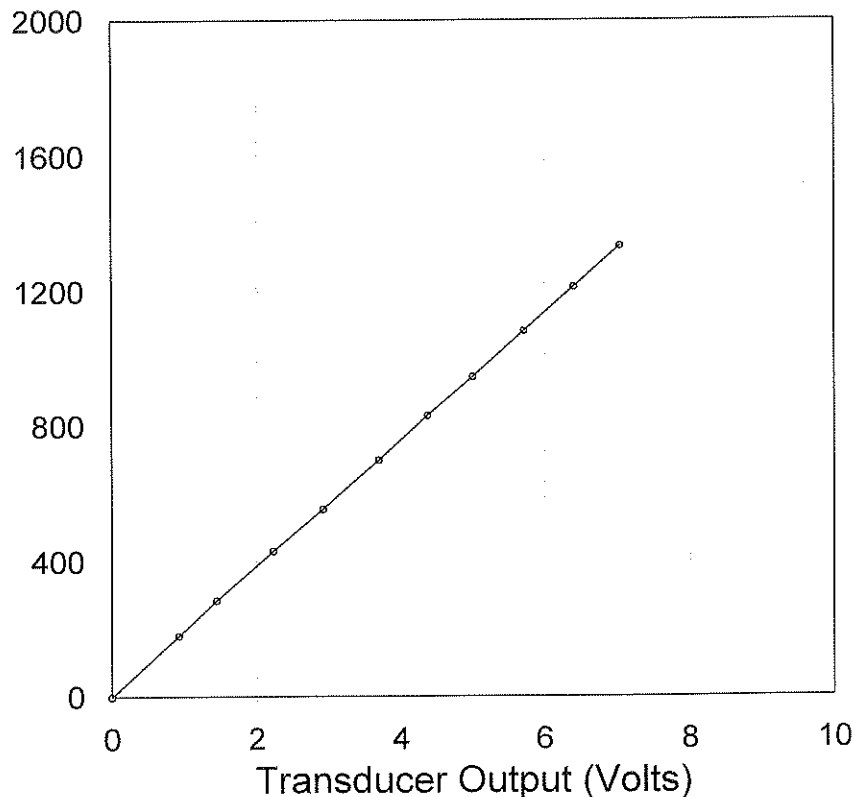

PDA Cal Factor (5.0 V)

94.3 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
181	0.91
285	1.44
429	2.23
554	2.92
697	3.69
829	4.38
946	5.00
1082	5.71
1214	6.40
1335	7.04

Shunt (60.4 K Ω)

2.5 V

General Factor

327.4 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

06-Mar-2012