




Pile Dynamics, Inc.

Transducer G549

Strain ($\mu\epsilon$)

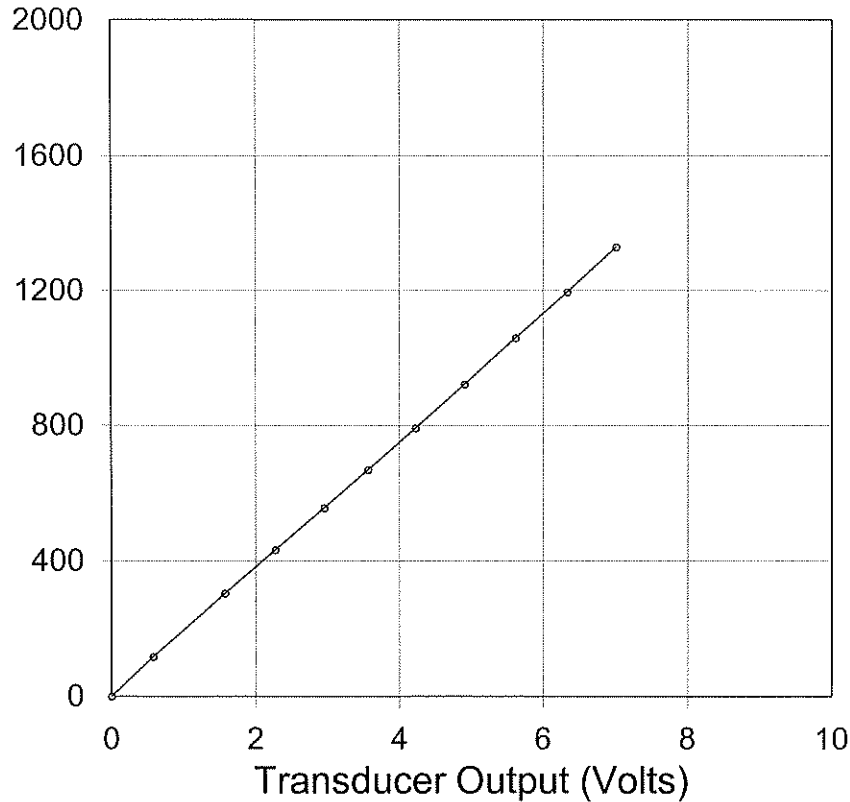

PDA Cal Factor (5.0 V)

94.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
119	0.58
303	1.57
431	2.27
556	2.95
668	3.56
791	4.22
921	4.90
1060	5.61
1197	6.33
1329	7.01

Shunt (60.4 K Ω)

2.5 V

General Factor

326.9 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

15-Apr-2011