


Pile Dynamics, Inc.

Transducer G825

Strain ($\mu\epsilon$)

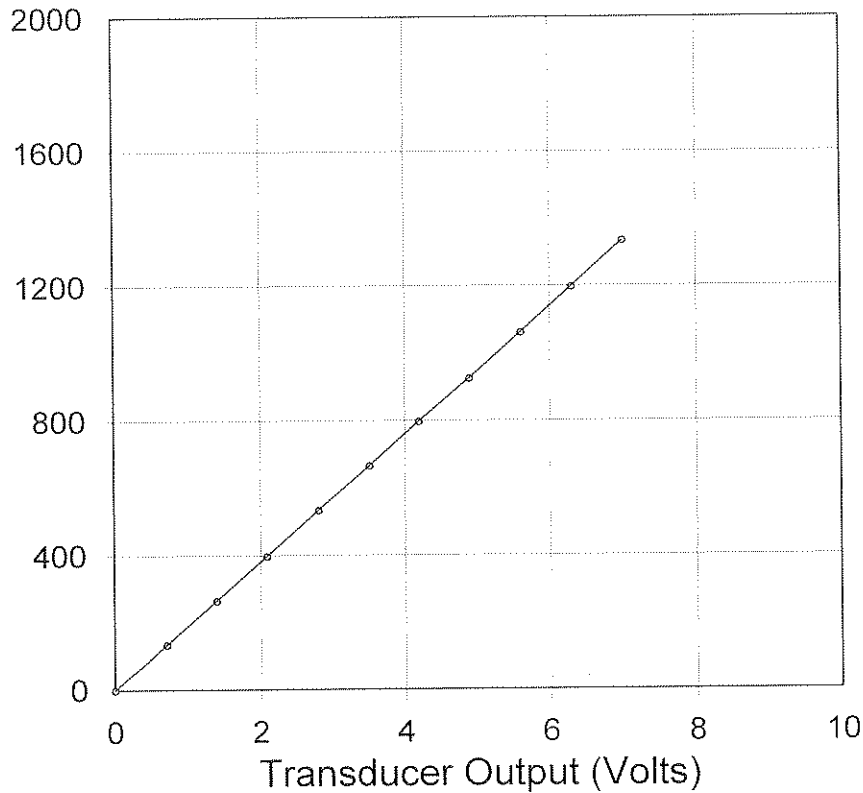

PDA Cal Factor (5.0 V) 95.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
136	0.70
266	1.39
397	2.09
534	2.81
665	3.51
797	4.19
926	4.89
1062	5.60
1199	6.30
1335	7.00

Shunt (60.4 K Ω) 2.5 V
 General Factor 330.2 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by: Kathleen Hillman
 Calibrated on: 07-Jul-2011

Smart Sensor? Yes No Smart Chip Programmed by: YH on: 7/7/11 CRC value 0697