




Pile Dynamics, Inc.

Transducer G834

Strain ($\mu\epsilon$)

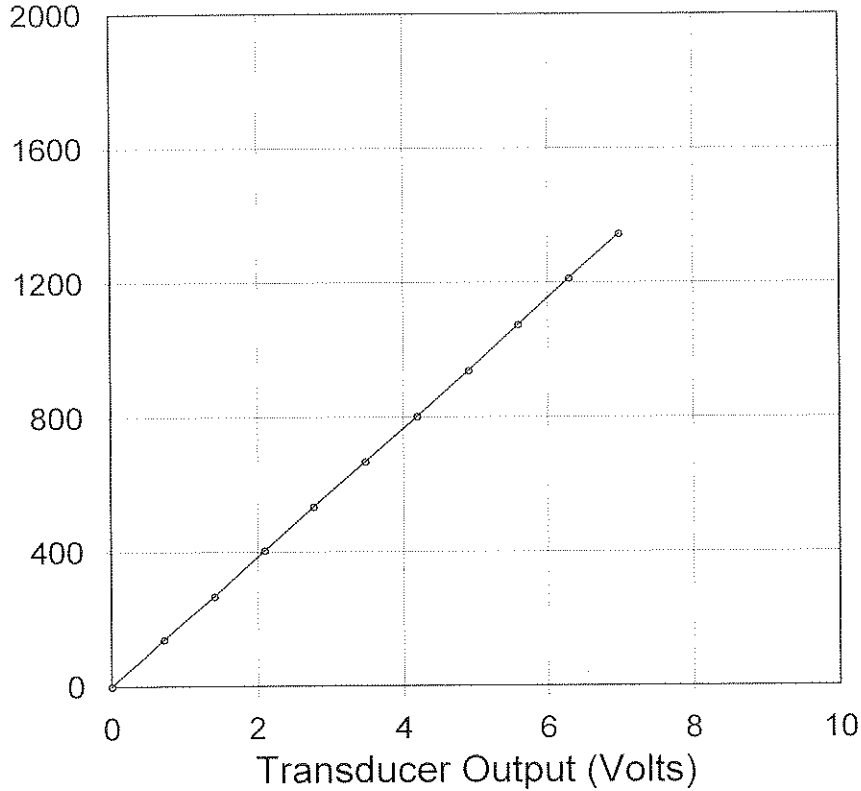

PDA Cal Factor (5.0 V)

96.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
139	0.70
268	1.40
404	2.10
534	2.78
668	3.48
802	4.18
938	4.90
1074	5.59
1213	6.30
1345	6.99

Shunt (60.4 K Ω)

2.5 V

General Factor

333.6 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Kathleen Hillman

Calibrated on:

07-Jul-2011

Strain Transducer Calibrator System 2009 Version 1.3

Smart Sensor? Yes No Smart Chip Programmed by: *KW* on: *7/7/11* CRC value *2E88*