




Pile Dynamics, Inc.

# Pile Dynamics, Inc.

## Transducer G835

Strain ( $\mu\epsilon$ )

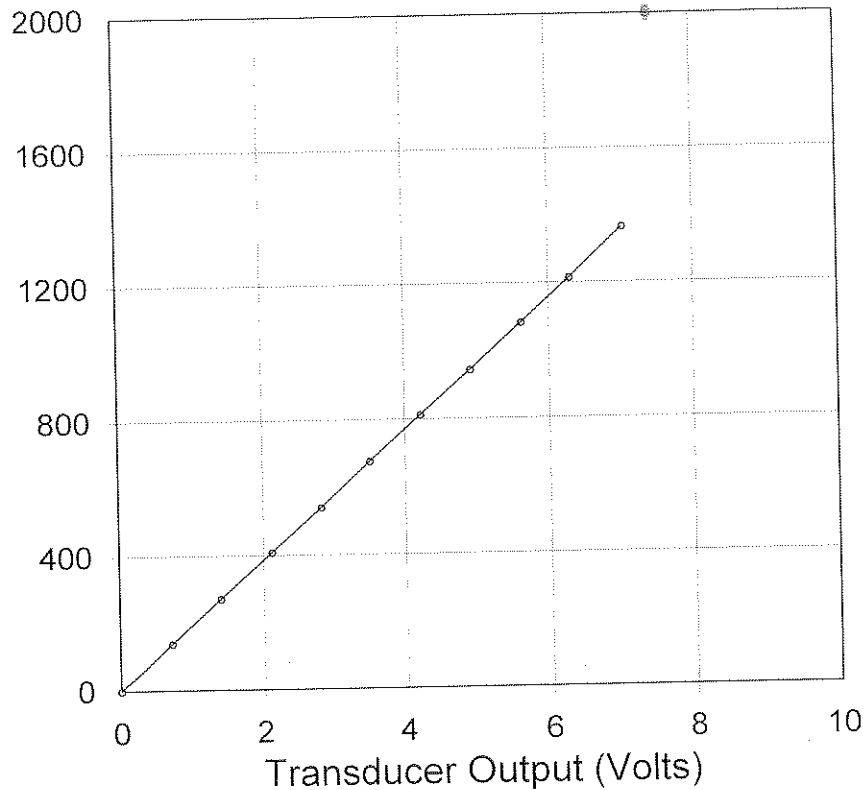

PDA Cal Factor (5.0 V)

96.6 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
139	0.71
273	1.40
409	2.12
541	2.82
677	3.51
813	4.22
945	4.91
1084	5.62
1215	6.29
1366	7.03

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

335.5 $\mu\epsilon/mV/V$

Calibrated by:

*Kathleen Hillman*

Calibrated on:

07-Jul-2011

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Smart Sensor?  Yes  No Smart Chip Programmed by: YU on: 7/7/11 CRC value 7C7A