




Pile Dynamics, Inc.

Pile Dynamics, Inc.

Transducer G836

Strain ($\mu\epsilon$)

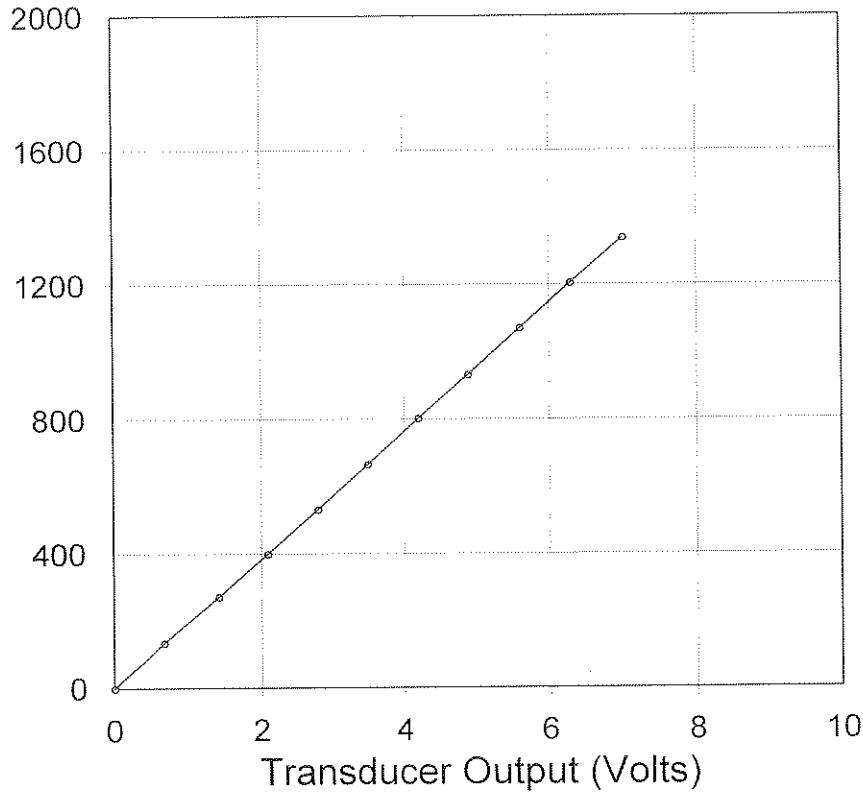

PDA Cal Factor (5.0 V)

95.3 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
136	0.67
273	1.41
400	2.09
531	2.79
665	3.49
802	4.20
931	4.89
1070	5.60
1203	6.29
1340	7.00

Shunt (60.4 K Ω)

2.5 V

General Factor

331.0 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by: Kathryn Hutton

Calibrated on: 07-Jul-2011

Strain Transducer Calibrator System 2009 Version 1.3

Smart Sensor? Yes No Smart Chip Programmed by: KH on: 7/7/11 CRC value 4884