Pile Dynamics, Inc.

Transducer G858

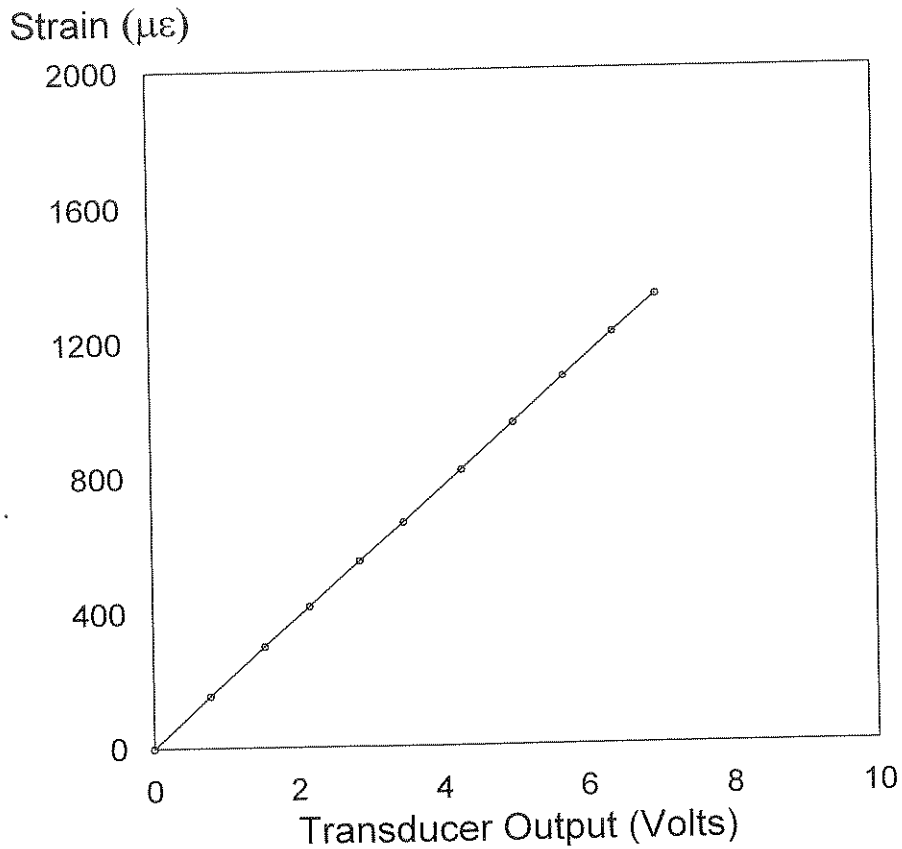

PDA Cal Factor (5.0 V) 95.0με/V

Applied Strain (με)	Transducer Output (Volts)
0	0.00
155	0.78
300	1.54
416	2.17
549	2.87
662	3.48
815	4.28
953	5.00
1089	5.70
1220	6.40
1330	6.99

Shunt (60.4 KΩ) 2.5 V

General Factor 329.7με/mV/V

Traceable to N.I.S.T.

Calibrated by: [signature]

Calibrated on: 06-Feb-2012

Strain Transducer Calibrator System 2011 Version 1.5

Smart Sensor? ✓ Yes ____ No Smart Chip Programmed by: VT on: 2-7-12 CRC value F9E0