


Pile Dynamics, Inc.

Transducer G860

Strain ($\mu\epsilon$)

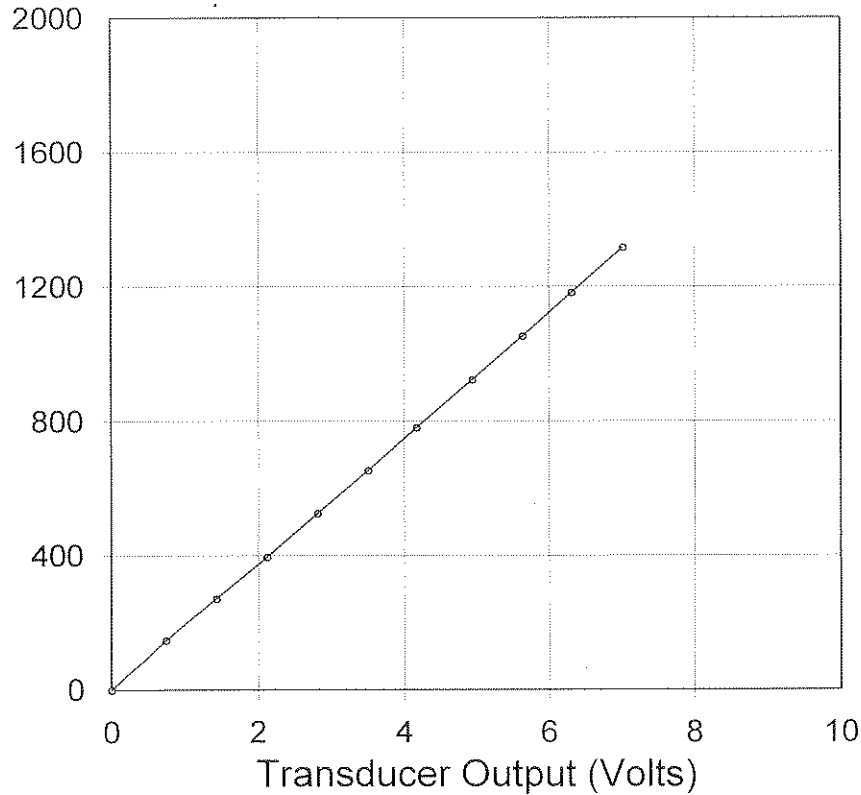

PDA Cal Factor (5.0 V)

93.3 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
148	0.73
272	1.42
396	2.12
525	2.80
653	3.50
780	4.17
923	4.94
1054	5.63
1183	6.31
1316	7.02

Shunt (60.4 K Ω)

2.5 V

General Factor

324.1 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by: Kathleen Hiltner

Calibrated on: 05-Jul-2011

Strain Transducer Calibrator System 2009 Version 1.3

Smart Sensor? Yes No Smart Chip Programmed by: KU on: 7/5/11 CRC value 10BB