


Pile Dynamics, Inc.

Transducer G861

Strain ($\mu\epsilon$)

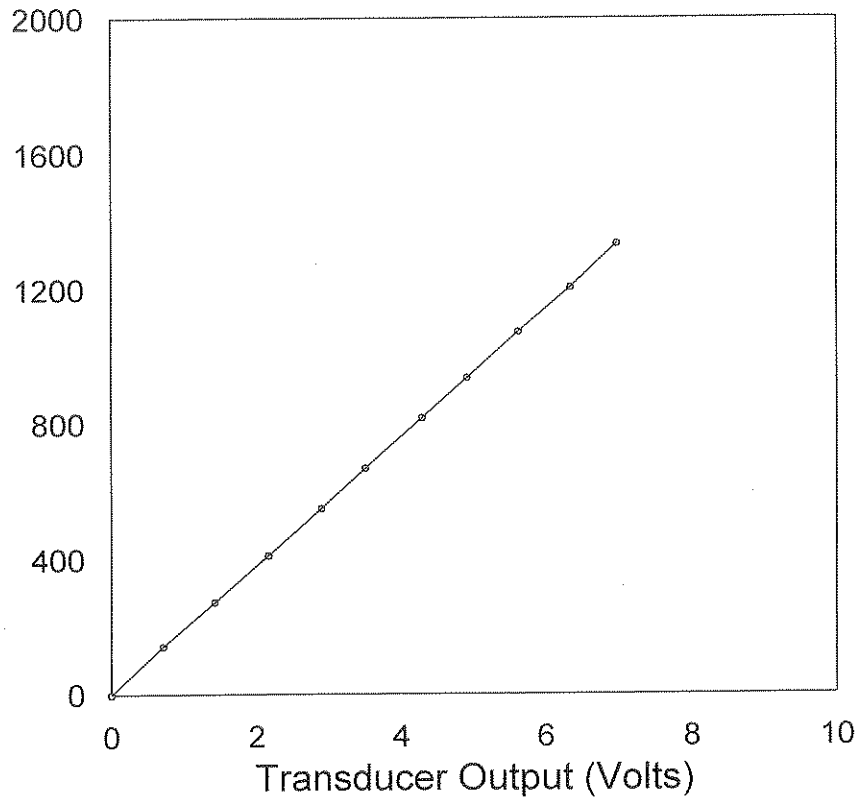

PDA Cal Factor (5.0 V)

95.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
145	0.70
273	1.41
410	2.16
549	2.89
668	3.50
817	4.29
935	4.91
1072	5.62
1206	6.33
1335	6.97

Shunt (60.4 K Ω)

2.5 V

General Factor

330.1 $\mu\epsilon/mV/V$

Calibrated by:

Ubach

Calibrated on:

28-Oct-2013

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Smart Sensor? Yes No Smart Chip

Programmed by: VT Date: 10-29-13 CRC value F0DF