




Pile Dynamics, Inc.

Transducer G862

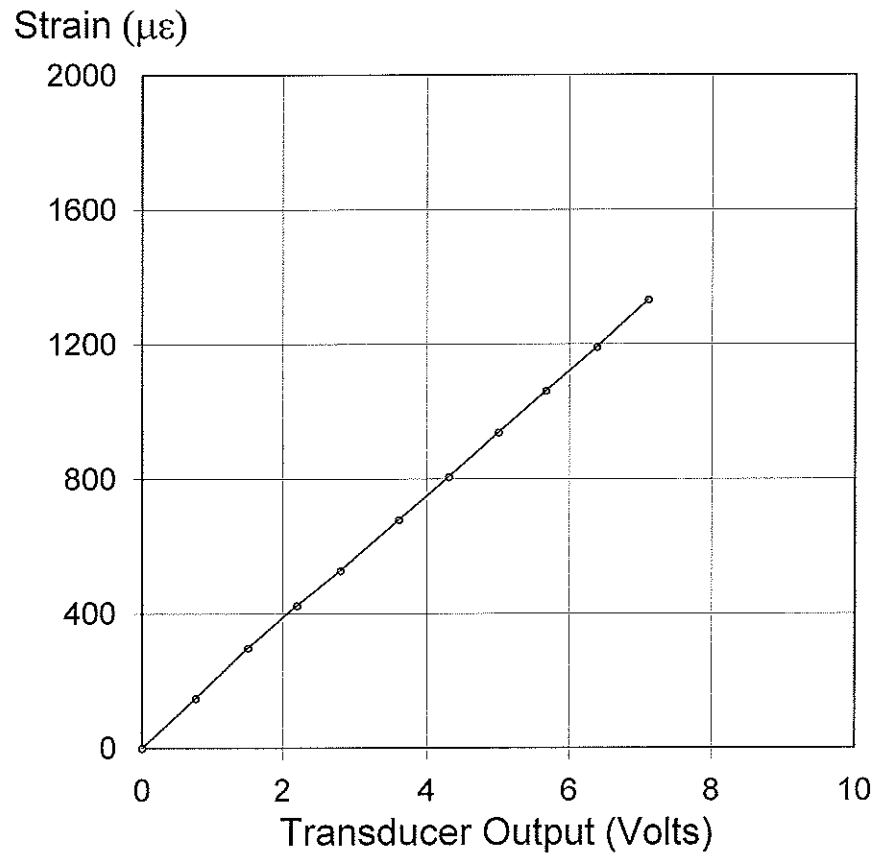

PDA Cal Factor (5.0 V) 93.0 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
148	0.76
298	1.50
423	2.19
526	2.80
678	3.61
806	4.30
938	5.00
1061	5.66
1192	6.38
1332	7.10

Shunt (60.4 K Ω) 2.5 V

General Factor 323.0 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by: [Signature]
 Calibrated on: 07-May-2012

Smart Sensor? Yes No Smart Chip Programmed by: VT Date: 5-8-12 CRC value HE81