




# Pile Dynamics, Inc.

## Transducer G897

Strain ( $\mu\epsilon$ )

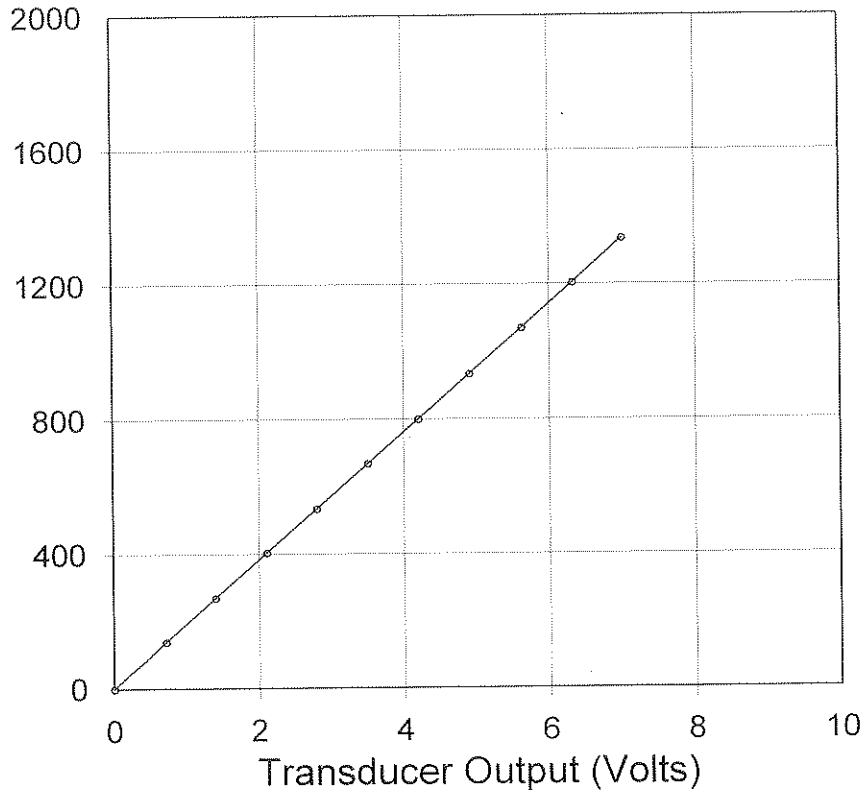

PDA Cal Factor (5.0 V)

95.1  $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
139	0.70
270	1.40
404	2.11
534	2.80
668	3.50
799	4.20
933	4.90
1070	5.62
1203	6.32
1337	7.00

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

330.3  $\mu\epsilon/mV/V$

Calibrated by:

*Kathleen Hutton*

Calibrated on:

07-Jul-2011

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Smart Sensor?  Yes  No Smart Chip Programmed by: KU on: 7/7/11 CRC value 0379