




Pile Dynamics, Inc.

Pile Dynamics, Inc.

Transducer G899

Strain ($\mu\epsilon$)

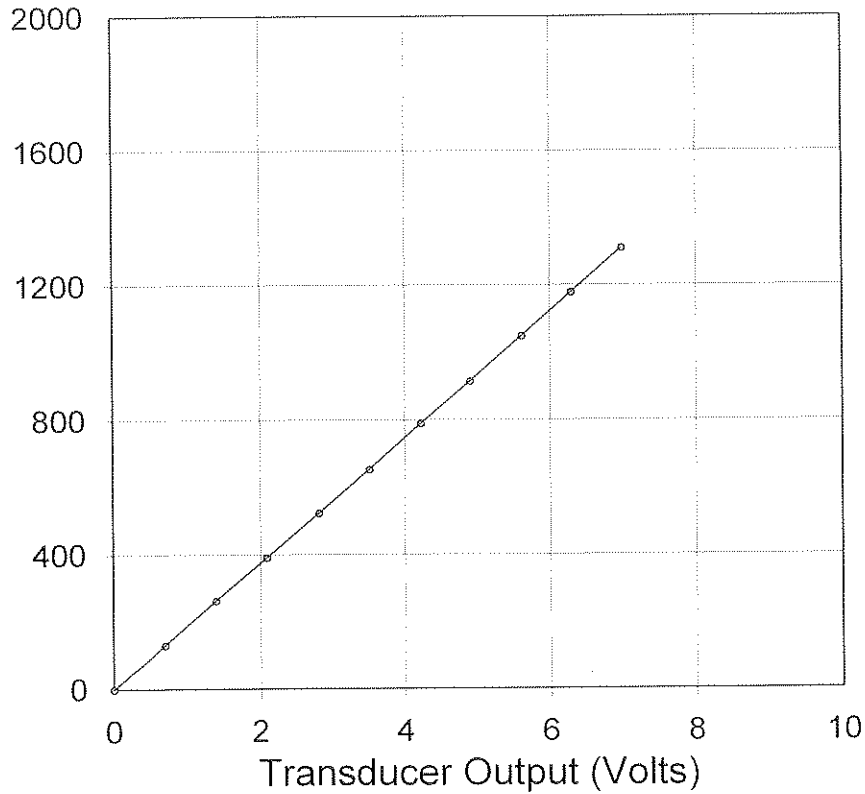

PDA Cal Factor (5.0 V)

93.5 $\mu\epsilon/V$

| Applied Strain ($\mu\epsilon$) | Transducer Output (Volts) |
|----------------------------------|---------------------------|
| 0 | 0.00 |
| 132 | 0.69 |
| 263 | 1.39 |
| 390 | 2.09 |
| 522 | 2.80 |
| 653 | 3.51 |
| 790 | 4.22 |
| 914 | 4.90 |
| 1048 | 5.61 |
| 1178 | 6.29 |
| 1312 | 6.99 |

Shunt (60.4 K Ω)

2.5 V

General Factor

324.8 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Kathleen Hallinan

Calibrated on:

07-Jul-2011

Strain Transducer Calibrator System 2009 Version 1.3

Smart Sensor? Yes No Smart Chip Programmed by: YW on: 7/7/11 CRC value 7F27