




Pile Dynamics, Inc.

Pile Dynamics, Inc.

Transducer

G902

Strain ($\mu\epsilon$)

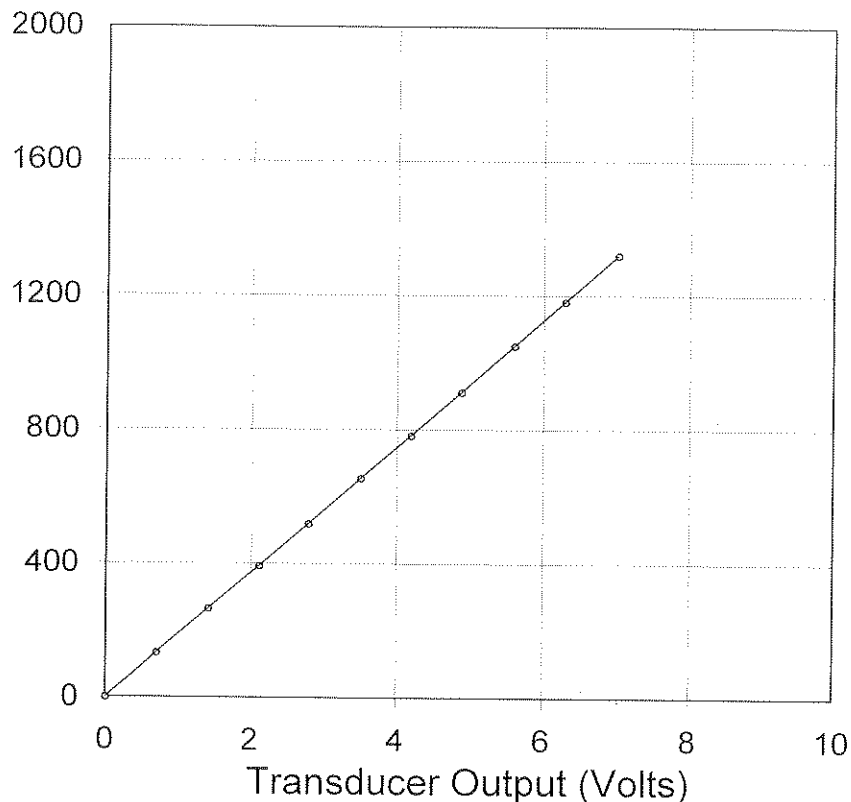

PDA Cal Factor (5.0 V)

93.9 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
134	0.69
266	1.40
393	2.11
519	2.78
656	3.50
783	4.19
912	4.88
1051	5.60
1182	6.29
1321	7.01

Shunt (60.4 K Ω)

2.5 V

General Factor

326.1 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Kaitlin Hiller

Calibrated on:

07-Jul-2011

Strain Transducer Calibrator System 2009 Version 1.3

Smart Sensor? Yes No Smart Chip Programmed by: YH on: 7/7/11 CRC value 8F1D