


Pile Dynamics, Inc.

Transducer G904

Strain ($\mu\epsilon$)

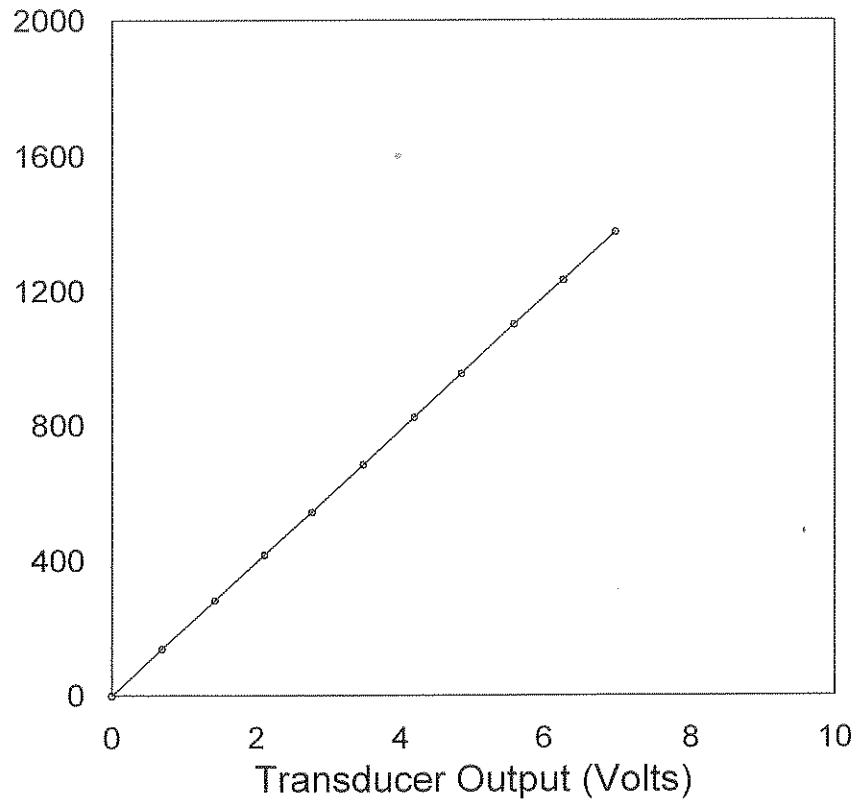

PDA Cal Factor (5.0 V)

98.4 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
141	0.69
282	1.42
416	2.11
543	2.77
683	3.48
824	4.19
953	4.85
1101	5.58
1234	6.26
1376	6.97

Shunt (60.4 K Ω)

2.5 V

General Factor

341.7 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by: *E. S. Saff*

Calibrated on:

24-Oct-2013

Smart Sensor? Yes No Smart Chip

Programmed by: E.S. Date: 10-24-13 CRC value 9774