


Pile Dynamics, Inc.

Pile Dynamics, Inc.

Transducer G906

Strain ($\mu\epsilon$)

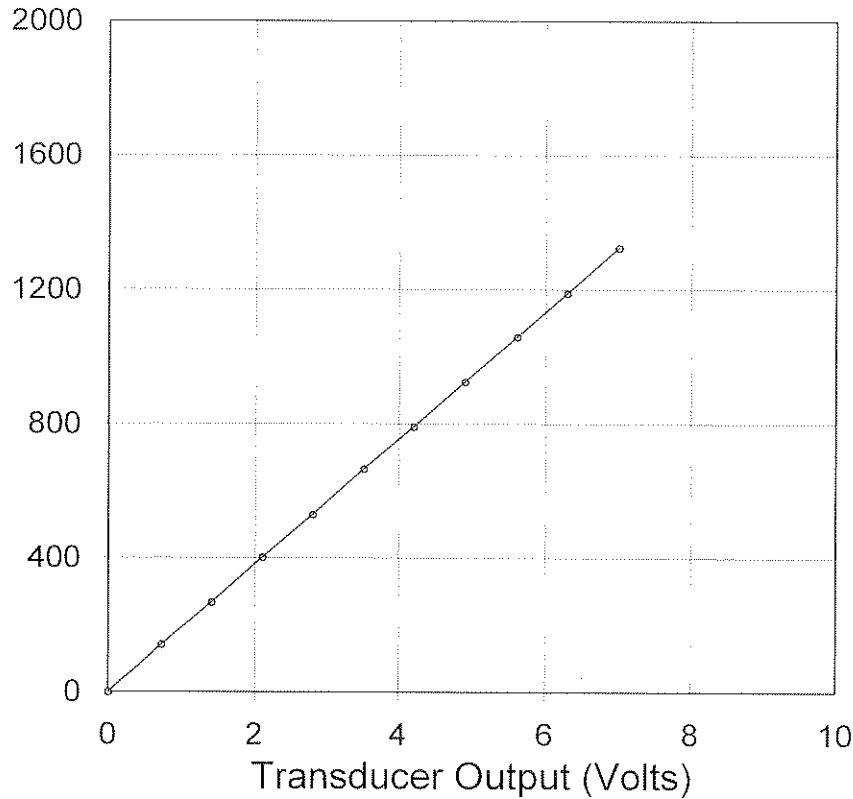

PDA Cal Factor (5.0 V)

94.3 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
141	0.71
282	1.39
423	2.10
564	2.80
705	3.51
846	4.20
987	4.90
1128	5.61
1269	6.29
1410	7.00

Shunt (60.4 K Ω)

2.5 V

General Factor

327.3 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by:

Kathleen Hillman

Calibrated on:

07-Jul-2011

Smart Sensor? Yes

No Smart Chip Programmed by:

YH

on: 7/7/11

CRC value

6390