




Pile Dynamics, Inc.

Transducer G907

Strain ($\mu\epsilon$)

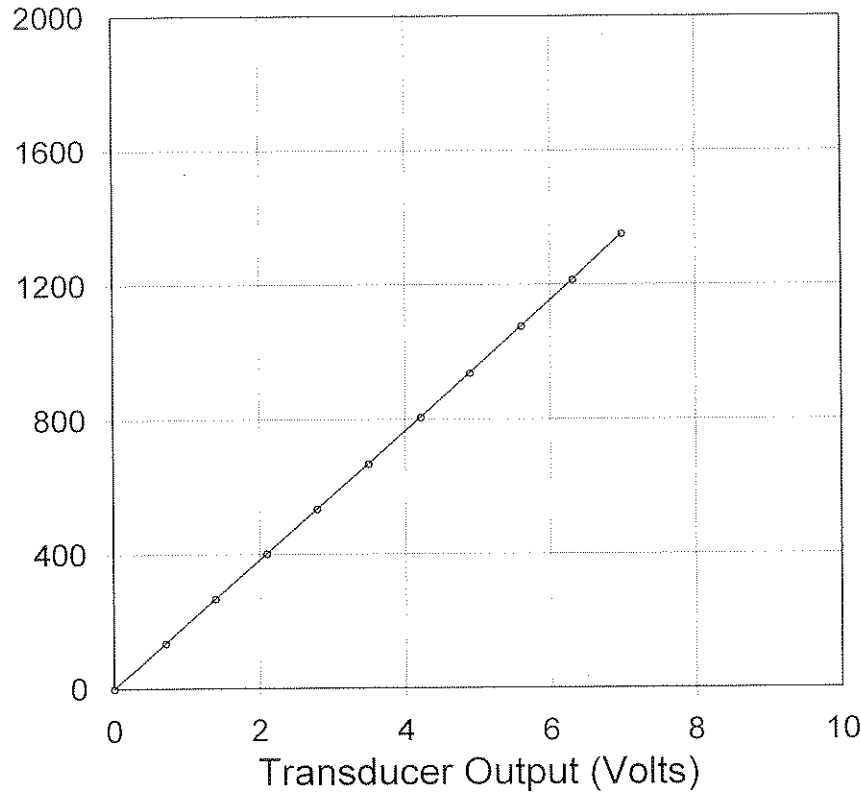

PDA Cal Factor (5.0 V)

96.4 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
136	0.70
268	1.39
402	2.10
534	2.79
668	3.49
806	4.20
938	4.89
1077	5.60
1215	6.31
1352	6.99

Shunt (60.4 K Ω)

2.5 V

General Factor

334.6 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Kathleen Hutton

Calibrated on:

07-Jul-2011

Strain Transducer Calibrator System 2009 Version 1.3

Smart Sensor? Yes No Smart Chip Programmed by: *YH* on: *7/7/11* CRC value *5C8D*