




Pile Dynamics, Inc.

Transducer H339

Strain ($\mu\epsilon$)

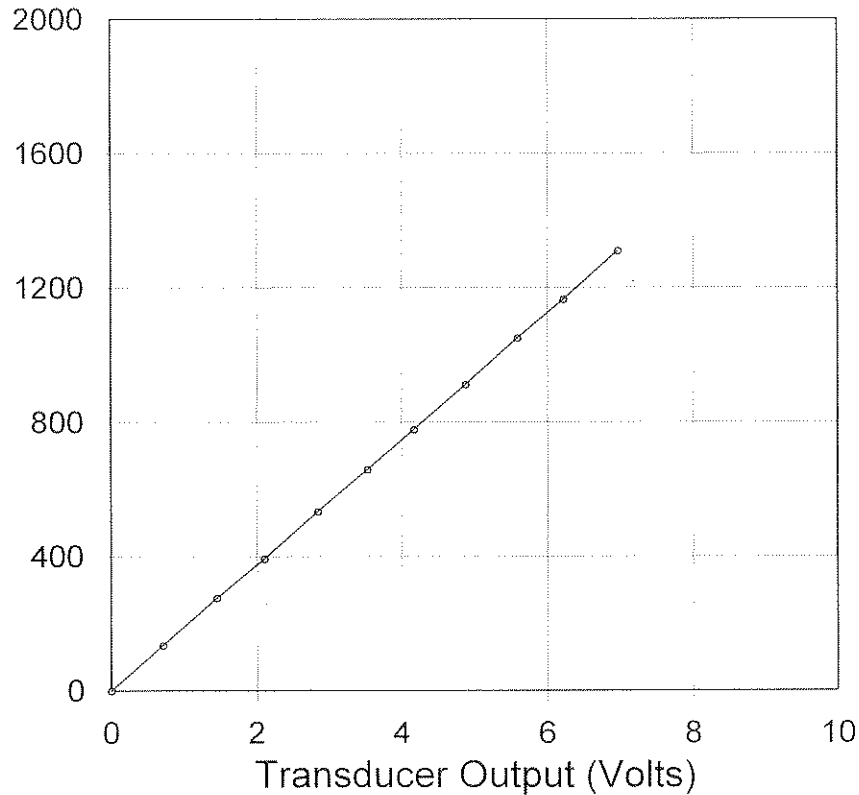

PDA Cal Factor (5.0 V)

93.7 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
135	0.71
276	1.45
393	2.10
533	2.84
658	3.53
779	4.17
912	4.88
1051	5.59
1165	6.21
1311	6.97

Shunt (60.4 K Ω)

2.5 V

General Factor

325.3 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Smart Sensor? Yes No Smart Chip

Calibrated by: Jenny Piesalko
 Calibrated on: 04-Jan-2012

Programmed by: JP on: 1-4-12 CRC value 551B