




Pile Dynamics, Inc.

Pile Dynamics, Inc.

Transducer

H341

Strain ($\mu\epsilon$)

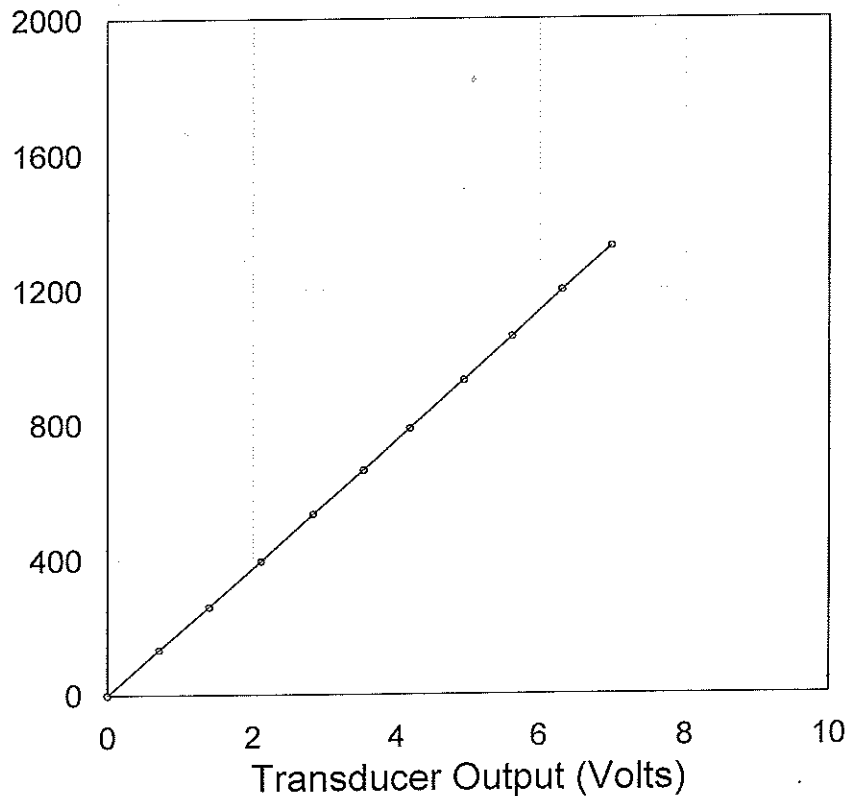

PDA Cal Factor (5.0 V)

94.8 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
136	0.70
262	1.39
396	2.11
534	2.83
664	3.53
787	4.18
930	4.93
1059	5.61
1197	6.31
1329	6.99

Shunt (60.4 K Ω)

2.5 V

General Factor

329.1 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by: *[Signature]*

Calibrated on:

07-Jan-2014

Smart Sensor? Yes No Smart Chip

Programmed by: E.S. Date: 1-7-14 CRC value 6F85