




Pile Dynamics, Inc.

Transducer H342

Strain ($\mu\epsilon$)

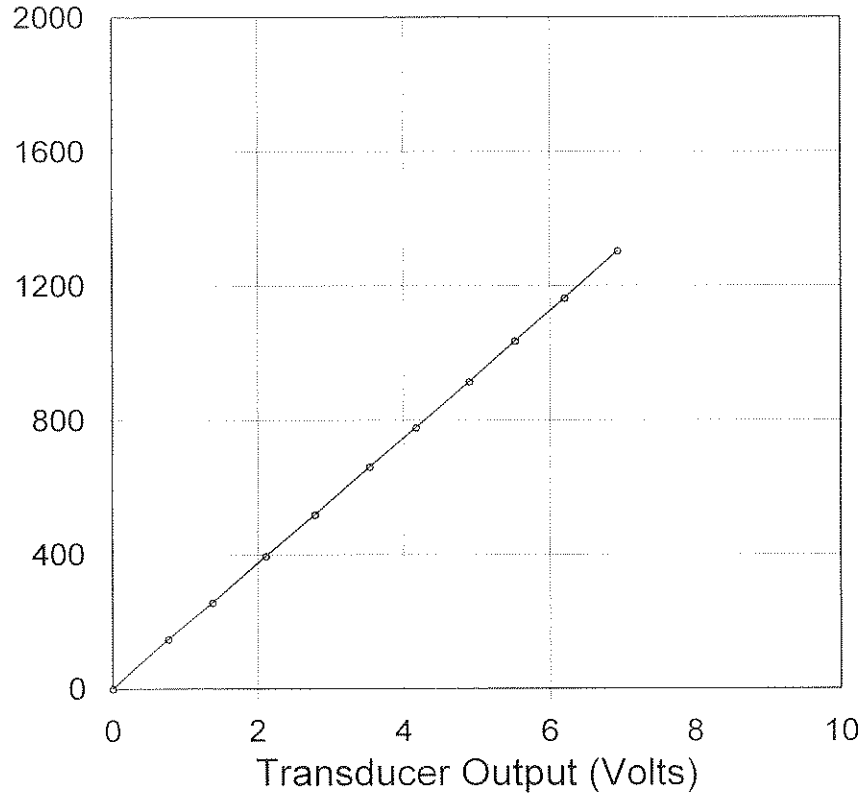

PDA Cal Factor (5.0 V)

93.7 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
148	0.76
296	1.37
444	2.11
592	2.78
740	3.53
888	4.17
1036	4.89
1184	5.53
1332	6.20
1480	6.93

Shunt (60.4 K Ω)

2.5 V

General Factor

325.5 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by: Jenny Piusalko

Calibrated on: 04-Jan-2012

Smart Sensor? Yes No Smart Chip

Programmed by: JP on: 1-4-12 CRC value 85E9