




# Pile Dynamics, Inc.

## Transducer H344

Strain ( $\mu\epsilon$ )

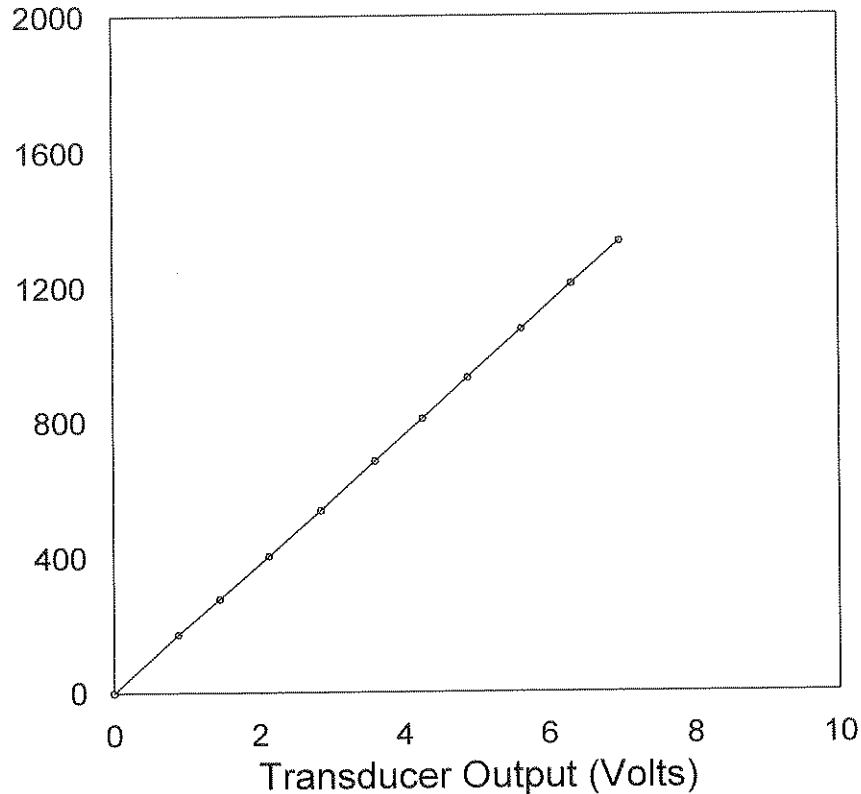

PDA Cal Factor (5.0 V)

95.3 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
174	0.87
277	1.45
403	2.13
537	2.85
682	3.60
808	4.26
929	4.89
1074	5.63
1208	6.32
1335	6.97

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

331.0 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by: *J. Stewart*

Calibrated on:

17-Jan-2012

Smart Sensor?  Yes  No Smart Chip

Programmed by: *VT* on: 1-17-12 CRC value FC91