


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

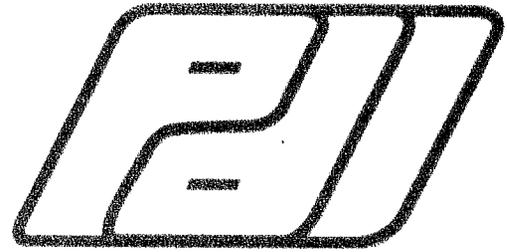

Serial No: K10768 Temperature: 22.3 °C
 Model: KICHER PR Humidity: 24%
 Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR
 421.2 mv/5000g
 (84.2 μv/g)
 R²: 0.999929 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
 1000 g's/volt
 Ref Acc 2: 85382! Cal on: 24Nov2025
 958 g's/volt


Operator: William Johnson

William Johnson
 Signed

Calibration valid 2 years

From: 25Feb2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

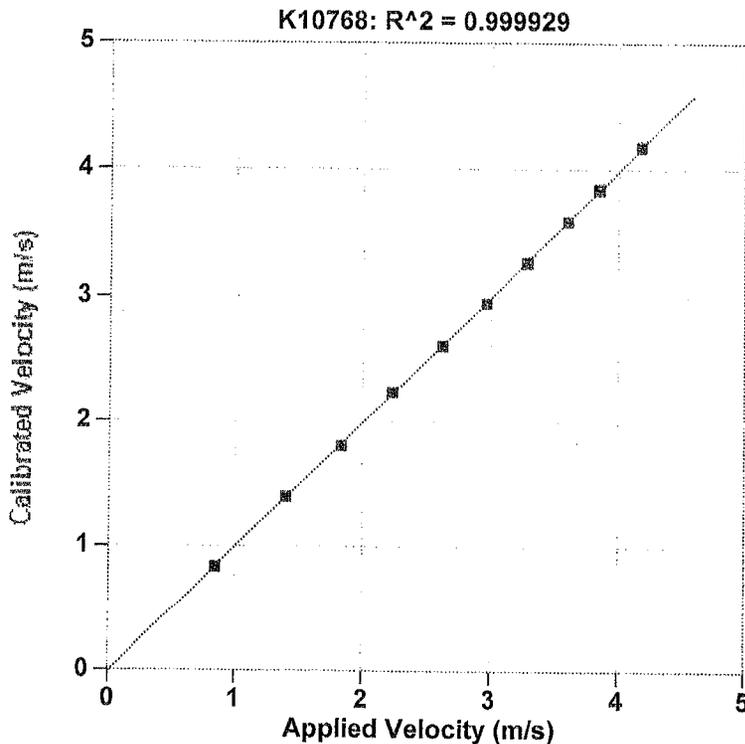

Reference Velocity	S/N K10768 Velocity
m/s	m/s
0.844	0.842
1.399	1.405
1.829	1.811
2.230	2.242
2.617	2.612
2.964	2.958
3.287	3.278
3.607	3.605
3.848	3.859
4.184	4.190

Maximum Acceleration: 903 g's