


# Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

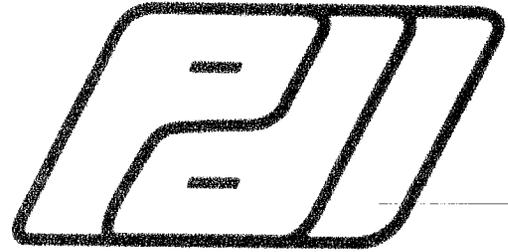

Serial No: K10770      Temperature: 22.3 °C

Model: KICHER PR      Humidity: 24%

Calibrated on: Channel 3 on 8G 5161 LE

### PDA CALIBRATION FACTOR

421.6 mv/5000g

(84.3 μv/g)

R<sup>2</sup>: 0.999942 [Chip programmed]

Ref Acc 1: 85363!      Cal on: 14Nov2025  
1000 g's/volt

Ref Acc 2: 85382!      Cal on: 24Nov2025  
958 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 25Feb2026

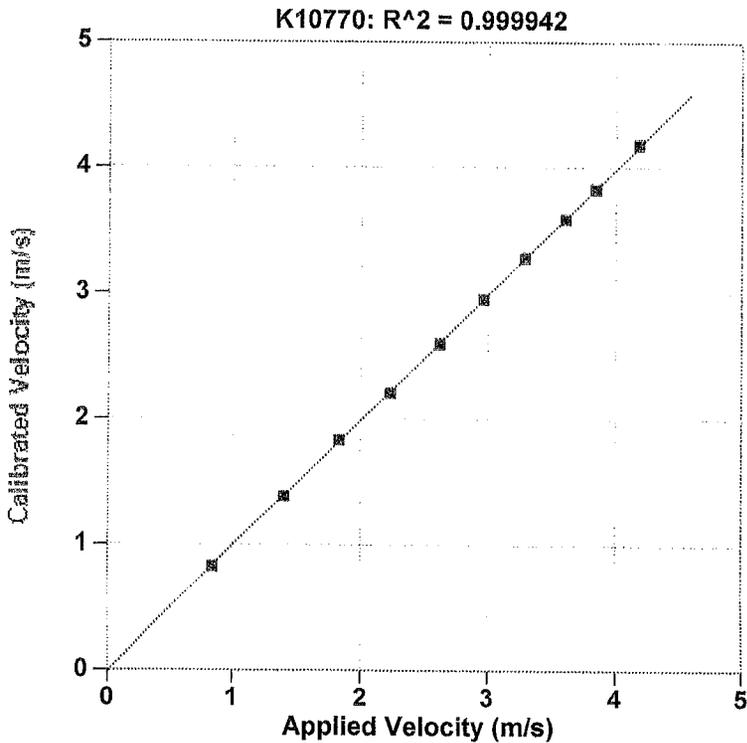

Reference Velocity	S/N K10770 Velocity
m/s	m/s
0.844	0.838
1.399	1.397
1.829	1.845
2.230	2.218
2.617	2.612
2.964	2.967
3.287	3.288
3.607	3.602
3.848	3.843
4.184	4.193

Maximum Acceleration: 903 g's