


# Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

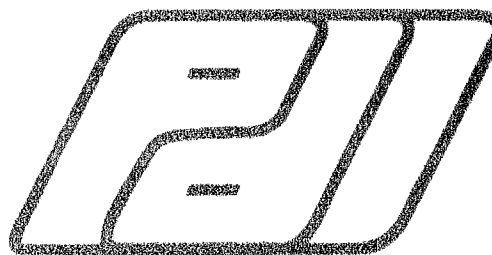

Serial No: K11960      Temperature: 22.5 °C  
 Model: KICHER PR      Humidity: 25%  
 Calibrated on: Channel 3 on 8G 5161 LE

**PDA CALIBRATION FACTOR**  
**376.8 mv/5000g**  
 (75.4  $\mu$ v/g)  
 R<sup>2</sup>: 0.999950 [Chip programmed]

Ref Acc 1: 85382!      Cal on: 24Nov2025  
 958 g's/volt  
 Ref Acc 2: 85363!      Cal on: 14Nov2025  
 1000 g's/volt


Operator: William Johnson

*William Johnson*  
 Signed

Calibration valid 2 years

From: 11Feb2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

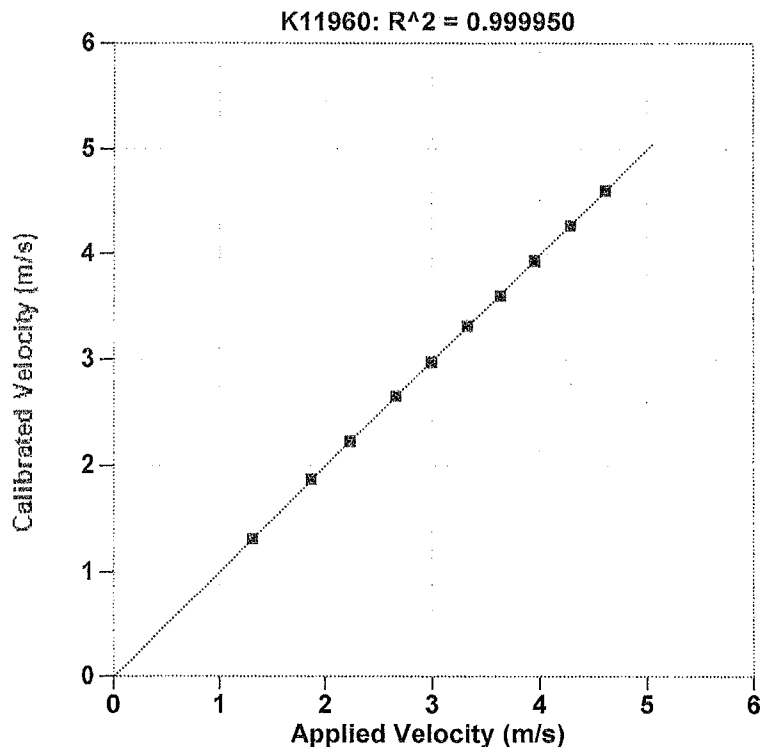

Reference Velocity	S/N K11960 Velocity
m/s	m/s
1.312	1.317
1.865	1.879
2.234	2.234
2.656	2.659
2.994	2.989
3.326	3.329
3.630	3.620
3.950	3.946
4.290	4.284
4.615	4.624

Maximum Acceleration: 1023 g's