


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

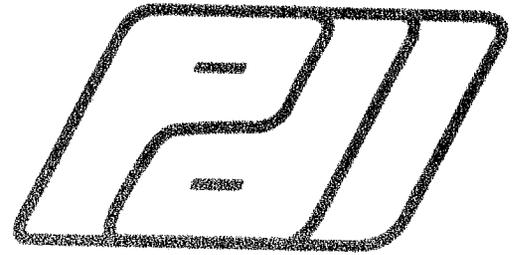

Serial No: K12480 Temperature: 20.3 °C
 Model: KICHER PR Humidity: 24%
 Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

454.7 mv/5000g
 (90.9 μ v/g)
 R²: 0.999946 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
 958 g's/volt
 Ref Acc 2: 85363! Cal on: 14Nov2025
 1000 g's/volt


Operator: William Johnson

William Johnson
 Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 14Mar2026

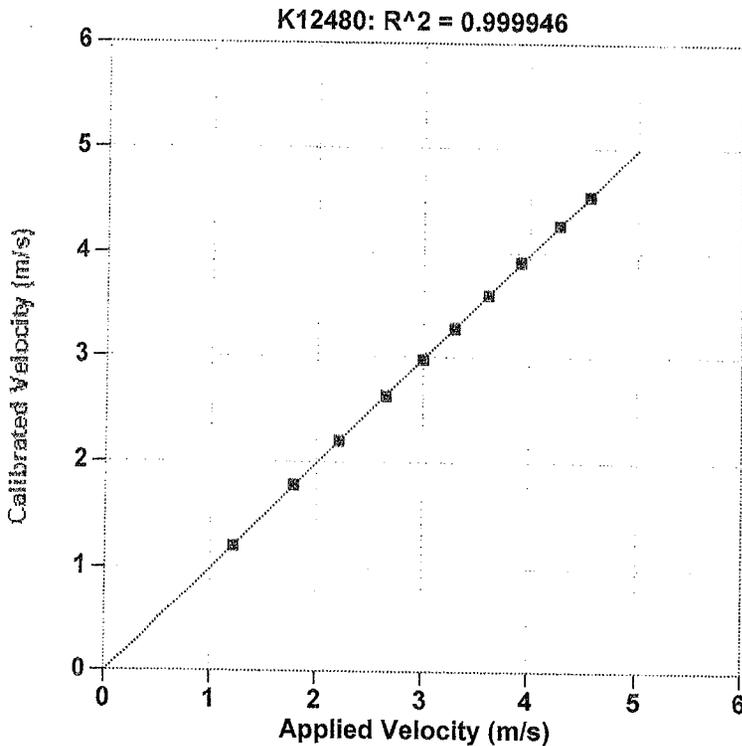

Reference Velocity	S/N K12480 Velocity
m/s	m/s
1.213	1.210
1.781	1.795
2.209	2.209
2.648	2.637
2.996	2.991
3.296	3.287
3.612	3.608
3.918	3.929
4.278	4.281
4.555	4.559

Maximum Acceleration: 966 g's