


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

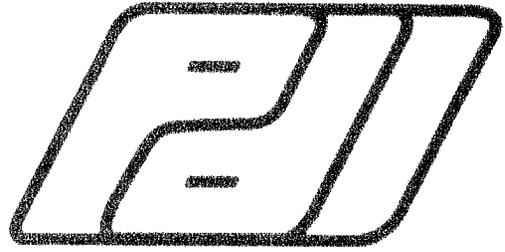

Serial No: K12908 Temperature: 23.0 °C
 Model: KICHER PR Humidity: 24%
 Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR
 448.4 mv/5000g
 (89.7 μv/g)
 R²: 0.999943 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
 1000 g's/volt
 Ref Acc 2: 85382! Cal on: 24Nov2025
 958 g's/volt


Operator: William Johnson

Signed

Calibration valid 2 years

From: 25Feb2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

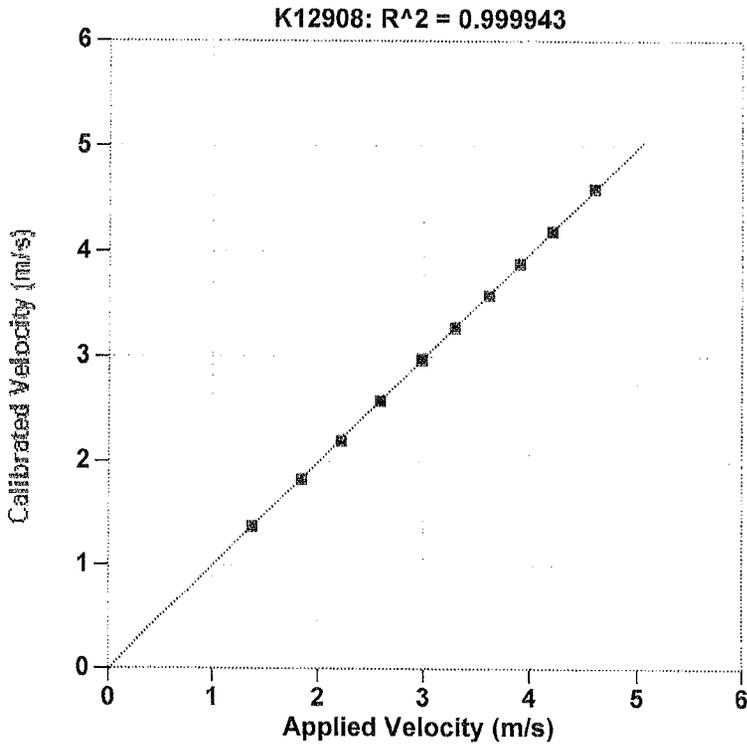

Reference Velocity	S/N K12908 Velocity
m/s	m/s
1.379	1.373
1.840	1.838
2.220	2.205
2.590	2.585
2.982	2.984
3.293	3.289
3.608	3.602
3.903	3.908
4.205	4.207
4.604	4.617

Maximum Acceleration: 995 g's