


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

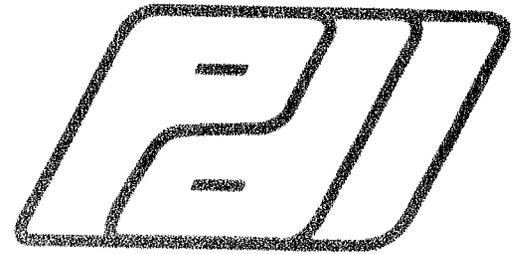

Serial No: K13554 Temperature: 20.3 °C
 Model: KICHER PR Humidity: 24%
 Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

368.2 mv/5000g
 (73.6 $\mu\text{v/g}$)
 R²: 0.999970 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
 958 g's/volt
 Ref Acc 2: 85363! Cal on: 14Nov2025
 1000 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 14Mar2026

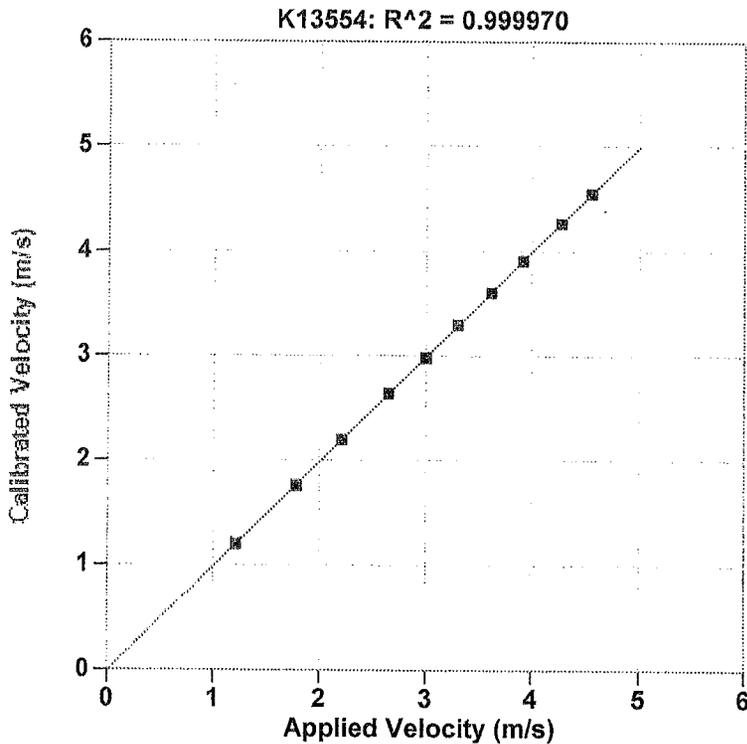

Reference Velocity	S/N K13554 Velocity
m/s	m/s
1.213	1.213
1.781	1.770
2.209	2.207
2.648	2.649
2.996	2.987
3.296	3.302
3.612	3.614
3.918	3.916
4.278	4.277
4.555	4.563

Maximum Acceleration: 966 g's