


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

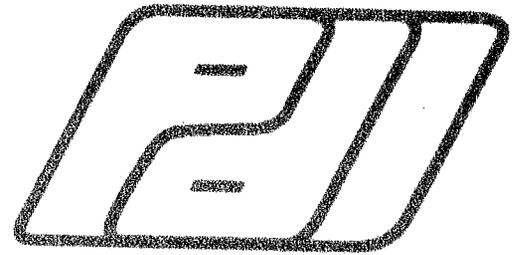

Serial No: K13555 Temperature: 20.3 °C
 Model: KICHER PR Humidity: 24%
 Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

400.6 mv/5000g
 (80.1 μ v/g)
 R²: 0.999904 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
 958 g's/volt
 Ref Acc 2: 85363! Cal on: 14Nov2025
 1000 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 14Mar2026

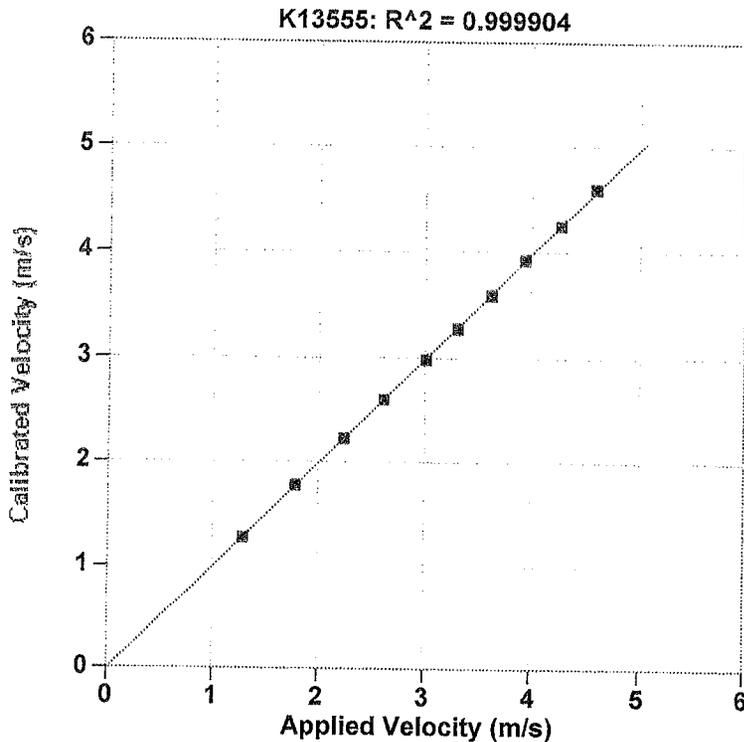

Reference Velocity m/s	S/N K13555 Velocity m/s
1.288	1.284
1.781	1.786
2.235	2.238
2.613	2.612
3.009	2.997
3.307	3.295
3.621	3.611
3.939	3.939
4.269	4.268
4.594	4.618

Maximum Acceleration: 973 g's