

Certificate of Calibration

Pile Dynamics, Inc.



Calibrated by Pile Dynamics, Inc.

Serial No: K15191 Temperature: 21.8 °C
 Model: KICHER PR Humidity: 23%
 Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

423.0 mv/5000g
 (84.6 μ v/g)
 R²: 0.999950 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
 1000 g's/volt
 Ref Acc 2: 85382! Cal on: 24Nov2025
 958 g's/volt


Operator: William Johnson

William Johnson
 Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: MAR 25 2026

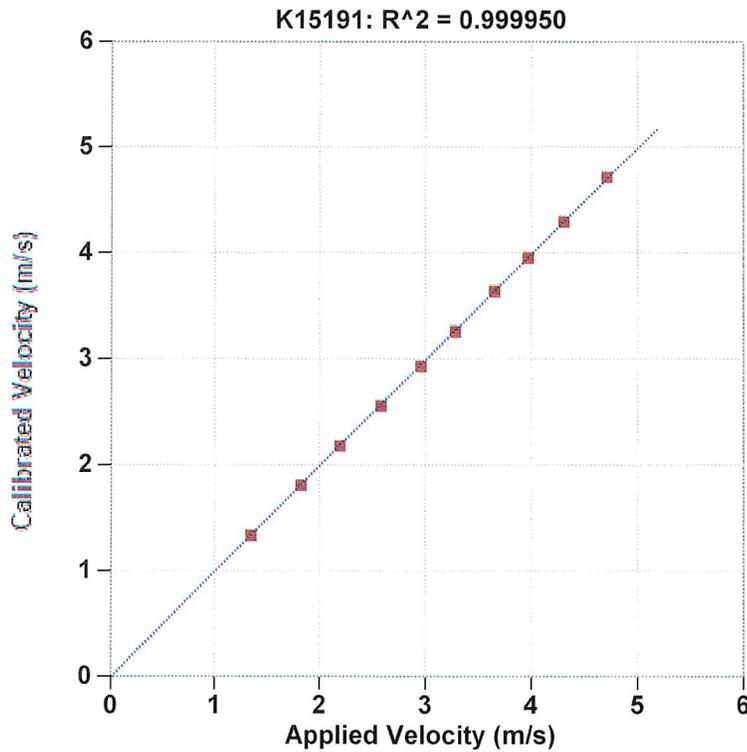

Reference Velocity	S/N K15191 Velocity
m/s	m/s
1.341	1.340
1.818	1.817
2.193	2.190
2.580	2.569
2.954	2.946
3.279	3.273
3.654	3.653
3.970	3.969
4.307	4.308
4.713	4.731

Maximum Acceleration: 1043 g's