


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

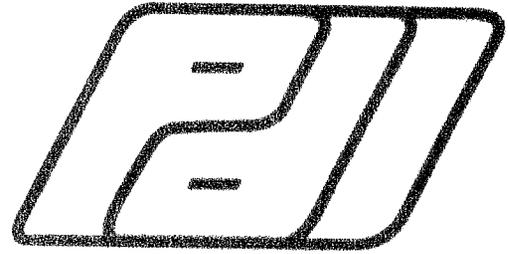

Serial No: K4230 Temperature: 22.5 °C

Model: KICHER PR Humidity: 24%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

455.6 mv/5000g

(91.1 μ v/g)

R²: 0.999903 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 25Feb2026

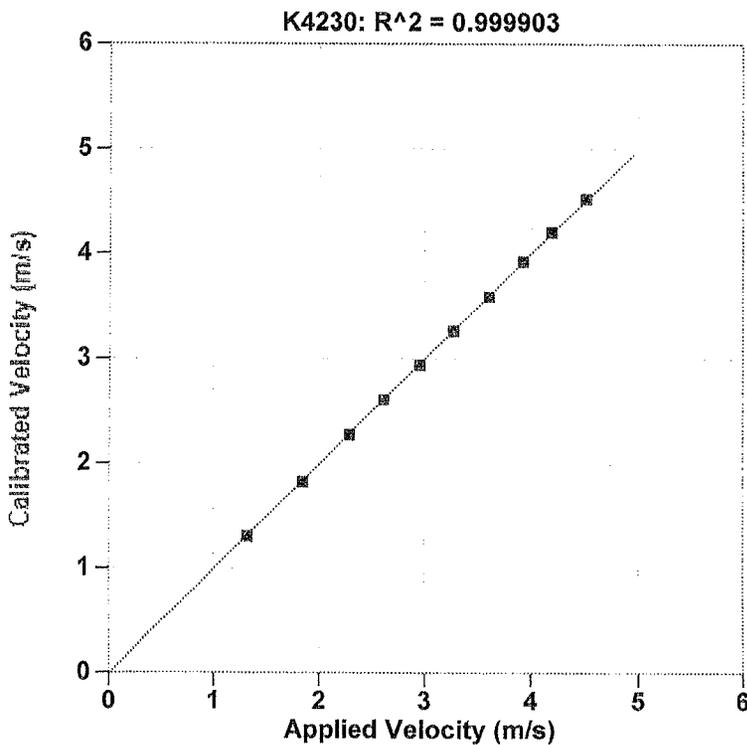

Reference Velocity	S/N K4230 Velocity
m/s	m/s
1.320	1.313
1.844	1.837
2.296	2.283
2.620	2.612
2.953	2.943
3.272	3.267
3.600	3.596
3.925	3.924
4.191	4.205
4.514	4.531
Maximum Acceleration: 979 g's	