


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

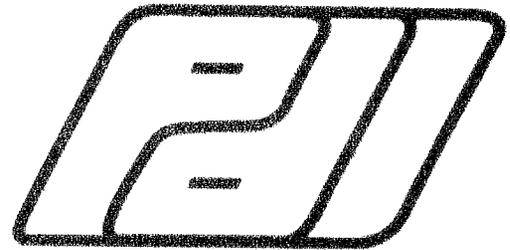

Serial No: K5485 Temperature: 22.1 °C
 Model: KICHER PR Humidity: 24%
 Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

349.3 mv/5000g
 (69.9 μ v/g)
 R²: 0.999983 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
 1000 g's/volt
 Ref Acc 2: 85382! Cal on: 24Nov2025
 958 g's/volt


Operator: William Johnson

William Johnson
 Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 25Feb2026

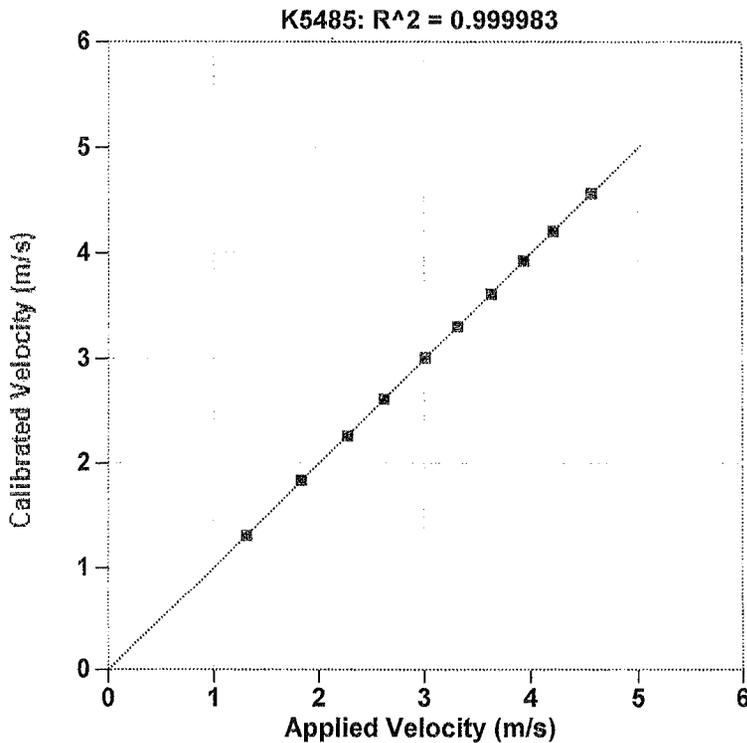

Reference Velocity	S/N K5485 Velocity
m/s	m/s
1.314	1.311
1.833	1.837
2.273	2.267
2.618	2.621
3.007	3.015
3.312	3.313
3.627	3.621
3.936	3.933
4.212	4.214
4.574	4.574

Maximum Acceleration: 993 g's