


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

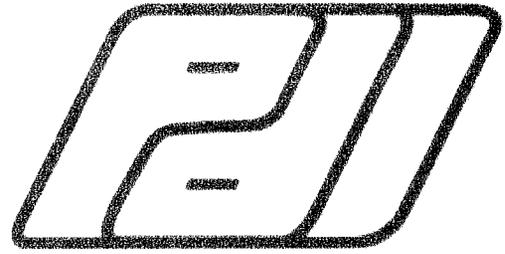

Serial No: K764 Temperature: 23.0 °C
 Model: KICHER PR Humidity: 24%
 Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

341.6 mv/5000g
 (68.3 μv/g)
 R²: 0.999965 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
 1000 g's/volt
 Ref Acc 2: 85382! Cal on: 24Nov2025
 958 g's/volt


Operator: William Johnson

Signed

Calibration valid 2 years

From: 25Feb2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

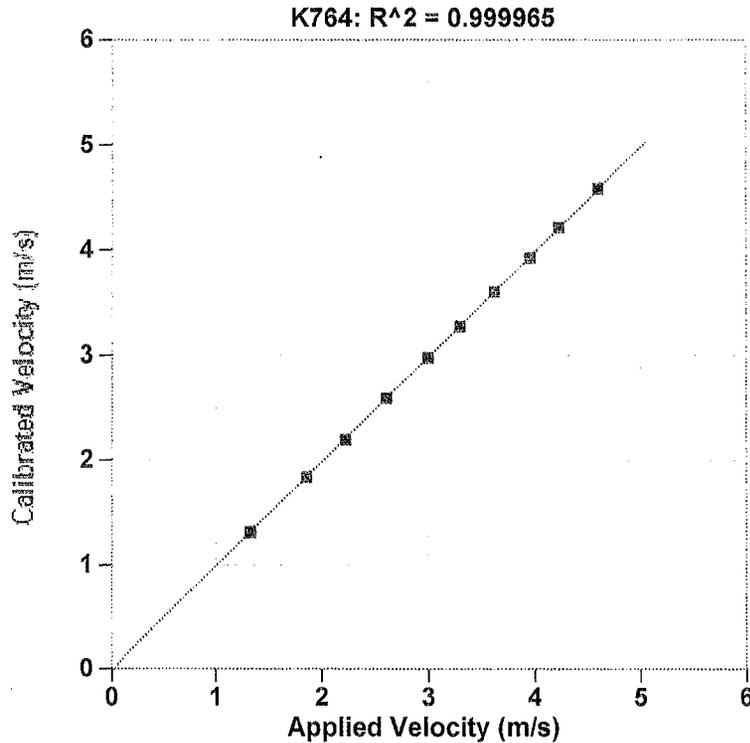

Reference Velocity	S/N K764 Velocity
m/s	m/s
1.326	1.325
1.852	1.847
2.218	2.206
2.605	2.600
2.993	2.991
3.292	3.290
3.619	3.623
3.951	3.946
4.228	4.235
4.594	4.603

Maximum Acceleration: 991 g's