

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: LW550191 Temperature: 22.1 °C
 Model: PIT ACC Humidity: 26%
 Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR
9.8 g's/volt
 R²: 0.999964 [Chip programmed]

Ref Acc 1: LW547723! Cal on: 21Oct2025
 10 g's/volt
 Ref Acc 2: LW547722! Cal on: 21Oct2025
 10 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: MAR 25 2026

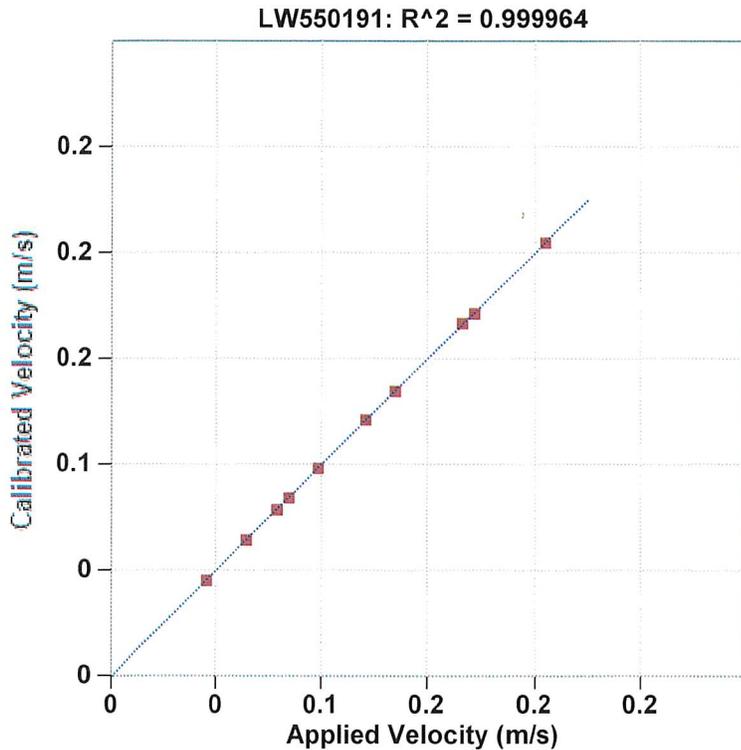

Reference Velocity	S/N LW550191 Velocity
m/s	m/s
0.045	0.045
0.064	0.064
0.079	0.079
0.084	0.084
0.098	0.098
0.121	0.121
0.135	0.135
0.166	0.167
0.172	0.172
0.205	0.205

Maximum Acceleration: 25 g's