




Pile Dynamics, Inc.

Transducer 1988

Strain ($\mu\epsilon$)

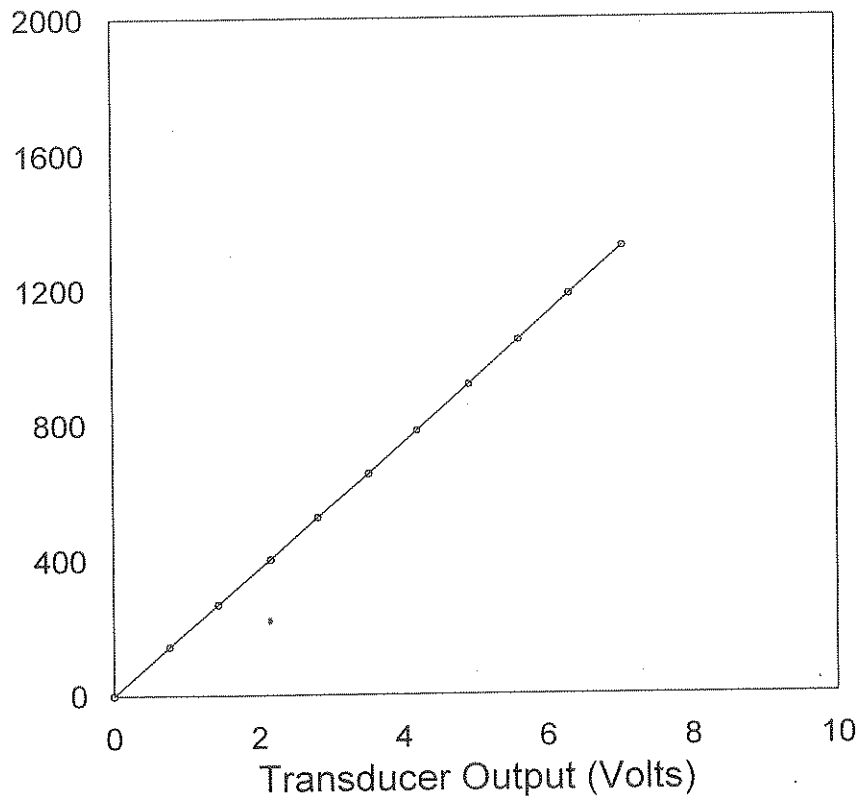

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

PDA Cal Factor (5.0 V)

93.7 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
146	0.76
271	1.43
402	2.16
524	2.82
653	3.53
780	4.20
918	4.92
1049	5.61
1184	6.31
1326	7.05

Shunt (60.4 K Ω)

2.5 V

General Factor

325.3 $\mu\epsilon/mV/V$

Calibrated by:

Calibrated on:

13-Feb-2014

Smart Sensor? Yes No Smart Chip

Programmed by: DB Date: 13-Feb-14 CRC value EEF5