




Pile Dynamics, Inc.

Transducer 1989

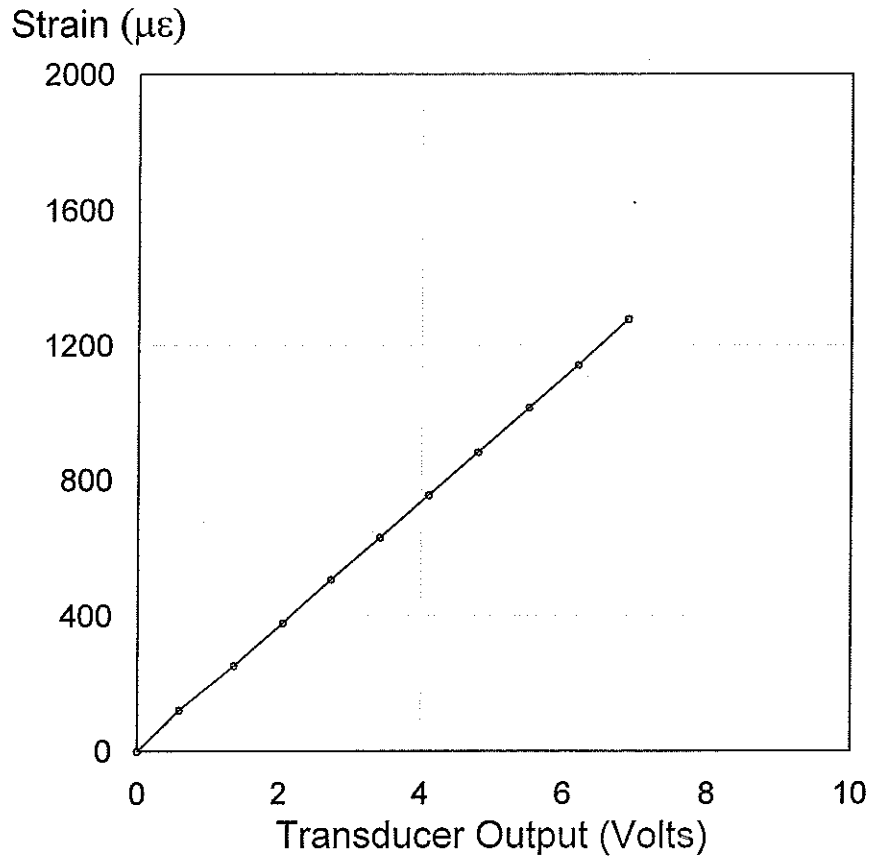

PDA Cal Factor (5.0 V) 92.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
123	0.58
252	1.36
378	2.05
505	2.73
630	3.42
754	4.09
882	4.79
1015	5.49
1142	6.18
1279	6.89

Shunt (60.4 K Ω) 2.5 V
 General Factor 319.8 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by: Jenny Piesalko
 Calibrated on: 28-Mar-2013

Smart Sensor? Yes No Smart Chip Programmed by: JP Date: 3-28-13 CRC value 3840