




Pile Dynamics, Inc.

Pile Dynamics, Inc.

Transducer

1991

Strain ($\mu\epsilon$)

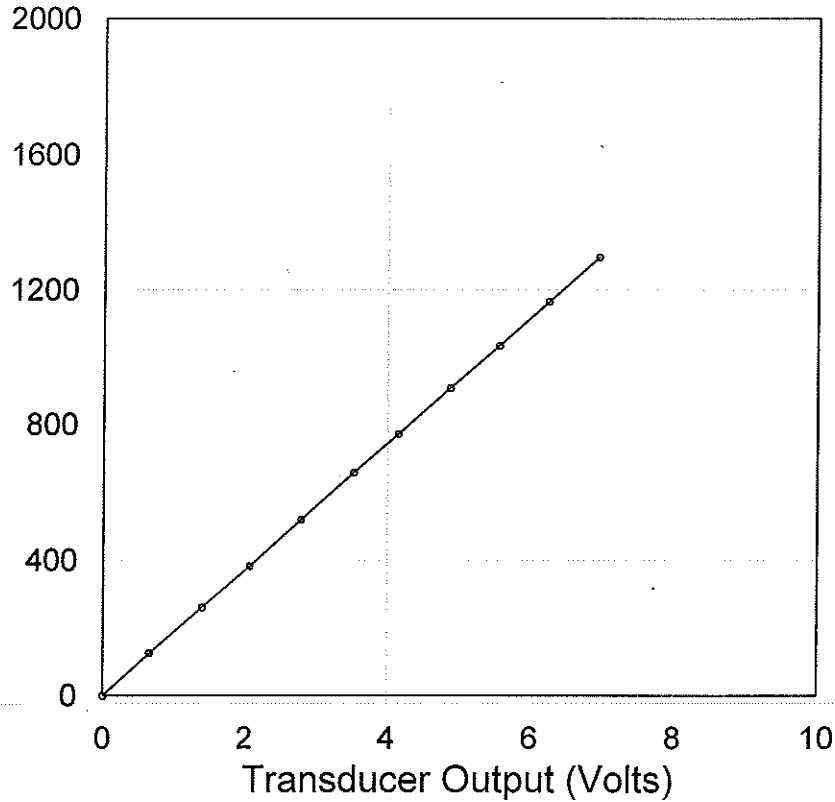

PDA Cal Factor (5.0 V)

93.2 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
127	0.65
260	1.39
382	2.06
518	2.78
656	3.52
771	4.15
907	4.87
1034	5.55
1165	6.24
1297	6.94

Shunt (60.4 K Ω)

2.5 V

General Factor

323.5 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by: Jenny Pisesalko

Calibrated on: 28-Mar-2013

Smart Sensor? Yes No Smart Chip Programmed by: JP Date: 3-28-13 CRC value CC38