


Pile Dynamics, Inc.

Transducer 1992

Strain ($\mu\epsilon$)

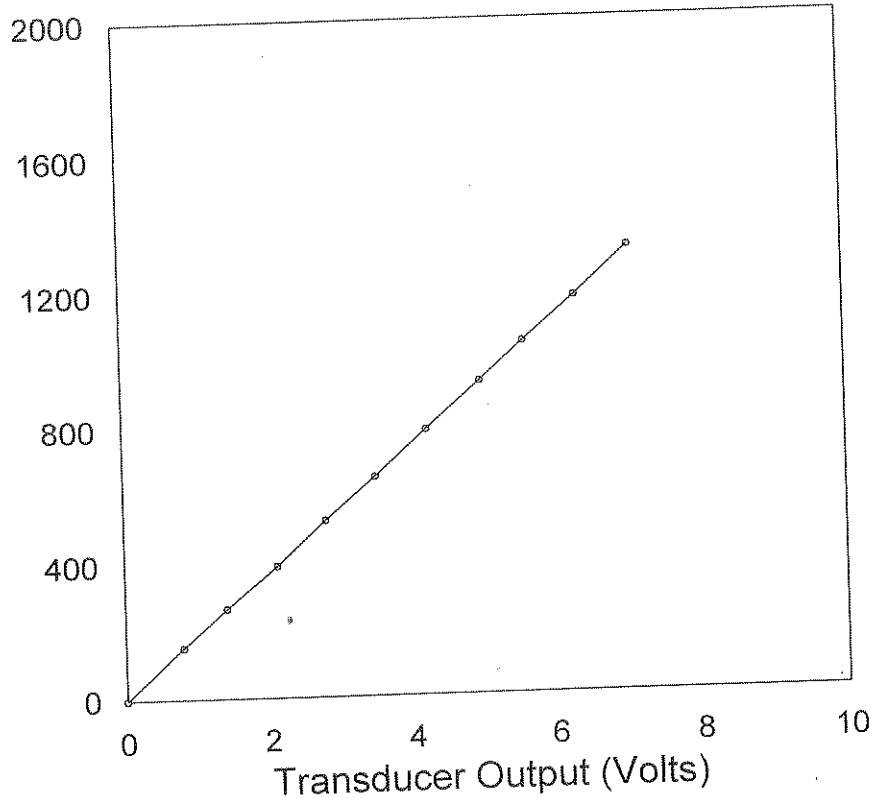

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

PDA Cal Factor (5.0 V) 93.0 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
155	0.79
267	1.40
390	2.11
524	2.79
649	3.49
784	4.21
924	4.97
1041	5.59
1174	6.31
1320	7.06

Shunt (60.4 K Ω) 2.5 V
 General Factor 322.8 $\mu\epsilon/mV/V$

Calibrated by: [Signature]
 Calibrated on: 26-Feb-2014

Smart Sensor? Yes No Smart Chip

Programmed by: E.S. Date: 2-26-14 CRC value 1058